

**Uitnodiging**

**Maandag 25 september 2023**

**Symposium voor Pathologie**

***On-slide controls for diagnostic IHC***  
**-**  
***IHC Critical Assay Performance Controls***

*Søren Nielsen,  
Director, NordiQC*



# Agenda and focus areas

- What is recommended and best practice for IHC controls in diagnostic IHC?
- What are the potentials and limitations for the use of IHC controls ?
- How can IHC controls be used by laboratories and IHC stakeholders?
  - How to use IHC controls to monitor assay consistency.
  - How to use IHC controls to address inter and intra test accuracy (e.g. EQA).

The role and concept behind ICAPCs -  
IHC Critical Assay Performance Controls  
Pros and cons..

- International IHC proficiency testing program
- Institute of Pathology, Aalborg University Hospital, Denmark
- About 670 participants from >60 countries



- General module: 3 runs/year
  - 15-17 different diagnostic markers (CDs, CKs, Transcrip.,...)
- Breast cancer IHC module: 2 runs/year
  - 3-5 different markers (HER2, ER, PR,...)
- HER-2 ISH module: 2 runs/year
  - BRISH, FISH (breast cancer)

- Companion (CDx) module: 2 runs/year
  - PD-L1 TPS/CPS – NSCLC/UC/TNBC (2017-)
  - PD-L1 IC score – TNBC/UC (2019-)



The screenshot shows the NordiQC website interface. At the top, there is a navigation bar with 'Info', 'Modules', 'Assessments', 'Protocols', 'Controls', 'Events', and 'Login'. Below this is a grid of four IHC images labeled A, B, C, and D. To the right of the images is a sidebar with 'Events' and 'Important dates' sections. Below the images is a text box with IHC results for PRAME in two laboratories. At the bottom right of the screenshot is the website URL 'www.nordiqc.org'.

**Events**

- NordiQC Workshop in Diagnostic Immunohistochemistry 2023  
4-6 Oct 2023; Aalborg, Denmark
- NordiQC Workshop in Diagnostic Immunohistochemistry 2024  
2-4 Oct 2024; Aalborg, Denmark

**Important dates**

- Run 69, B36, H24, C14  
Protocol submission deadline  
1 Sep 2023  
Slide circulation  
5 Sep 2023  
Slide return deadline  
10 Oct 2023  
Publication of results  
10 Dec 2023

**Questions**

Check out our [FAQ](#) (Frequently asked questions) or [contact us](#)

**IHC for PRAME in two laboratories:**

**Lab 1 (A+C):** Optimal results in testis (A) and malignant melanoma (C). In the testis, dispersed spermatogonia show a strong nuclear staining reaction, while nuclei of most spermatocytes a weak to moderate intensity. Leydig cells show a weak membranous staining reaction. In melanoma, virtually all neoplastic cells show a distinct moderate nuclear staining reaction.


**Lab 2 (B+D):** Insufficient result. In the testis (B), only few spermatogonia are demonstrated while spermatocytes and Leydig cells being negative. Only dispersed neoplastic cells of the melanoma (D) show a weak and equivocal nuclear staining reaction.

**Results - Run 68, C13**

10-Jul-2023  
The results for the runs 68 and C13 are now available on the website. Individual results can be seen after logging in. Protocol submission for next runs is open now and deadline is 1<sup>st</sup> of September.  
Please note, PRAME will be repeated in 2024. Therefore, no reassessment will be available.

[All news](#)

[www.nordiqc.org](http://www.nordiqc.org)

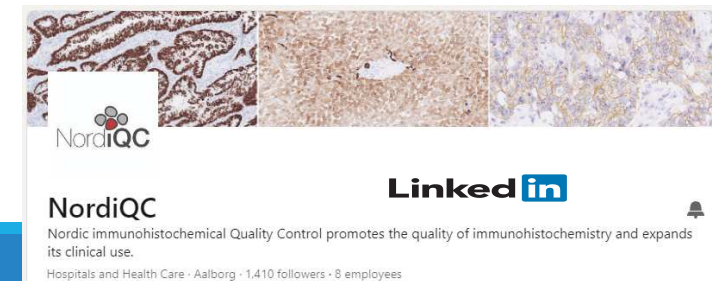

The screenshot shows the NordiQC LinkedIn profile page. At the top, there is a banner image with the NordiQC logo and the text 'Nordic immunohistochemical Quality Control promotes the quality of immunohistochemistry and expands its clinical use.' Below the banner is the NordiQC logo and the text 'Nordic immunohistochemical Quality Control promotes the quality of immunohistochemistry and expands its clinical use.' At the bottom, there is the text 'Hospitals and Health Care · Aalborg · 1,410 followers · 8 employees'.

**NordiQC**

Nordic immunohistochemical Quality Control promotes the quality of immunohistochemistry and expands its clinical use.


Hospitals and Health Care · Aalborg · 1,410 followers · 8 employees

## NordiQC assessment scheme 2024


Module	Winter	Spring	Autum
General*	<b>Run 70</b> <u>PRAME CGA p53</u> <u>Bcl-6 GATA3</u>	<b>Run 71</b> <u>INSM1 CD20</u> <u>PMS2 BAP1 Ki67</u> <u>CD117</u>	<b>Run 72</b> <u>TRPS1 CD8 MSH6</u> <u>p16 CK-PAN</u>
Breast*	<b>Run B37</b> <u>HER2 IHC ER PR</u>		<b>Run B38</b> <u>ER HER2 IHC</u>
HER2 ISH	<b>Run H25</b> <u>HER2 ISH</u>		<b>Run H26</b> <u>HER2 ISH</u>
Companion*		<b>Run C15</b> <u>PD-L1 (TPS/CPS)</u> <u>PD-L1 (IC)</u>	<b>Run C16</b> <u>PD-L1 (TPS/CPS)</u> <u>PD-L1 (IC)</u>

\*Accredited by DANAK under registration number 616 to proficiency testing.

... The IHC biomarker protocol trap – Caution: not for faint-hearted lab personel !!!!!

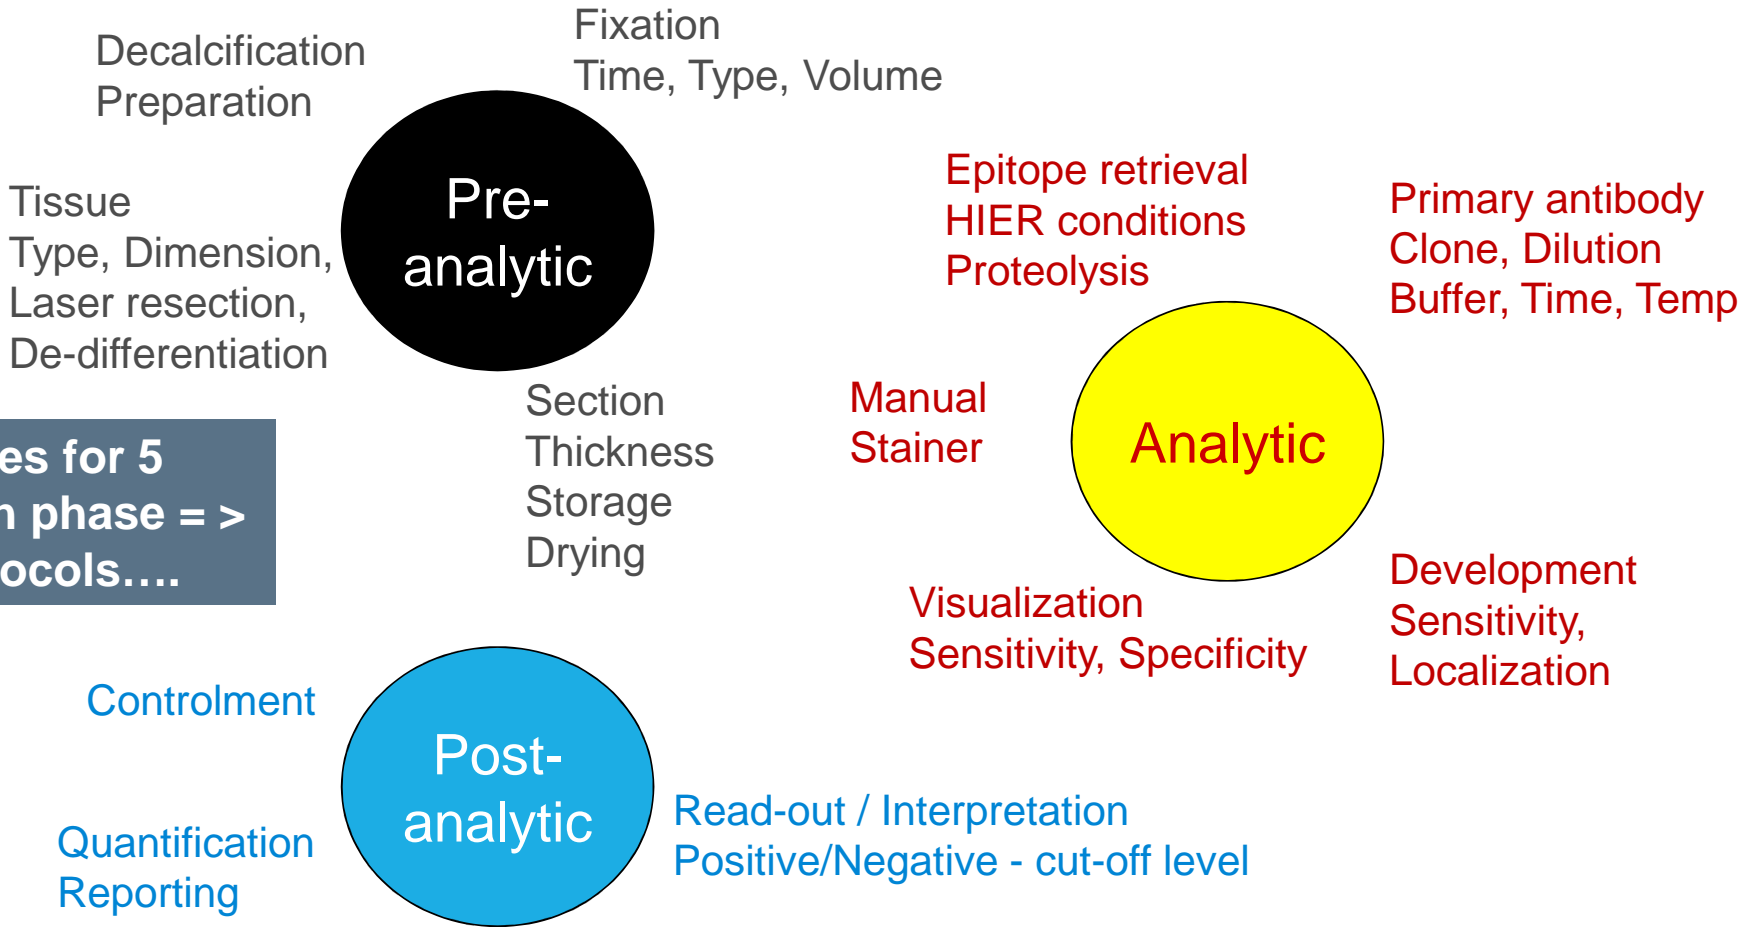

With 3 choices for 5 variables in each phase => 4 million protocols....

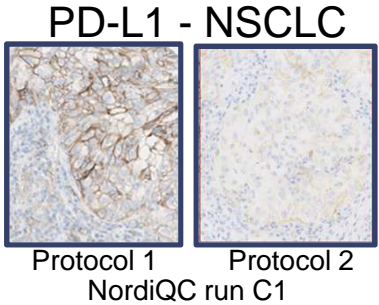


The use of the right controls at the right way can show if an IHC is right or wrong 😊

# Importance of IHC controls have been neglected....

## Documentation of *Diagnostic Cytopathology, Vol 39, No 4 2011* Immunocytochemistry Controls in the Cytopathologic Literature: A Meta-Analysis of 100 Journal Articles

Carol Colasacco, M.L.I.S., S.C.T.(A.S.C.P.), C.T.(I.A.C.),<sup>1\*</sup> Sharon Mount, M.D.,<sup>1,2</sup>  
and Gladv

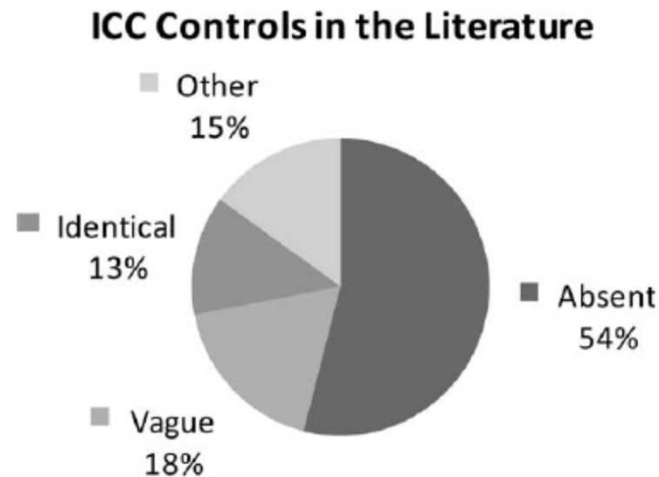

**Fig. 1.** Description of immunocytochemistry controls in articles reviewed.

Absent: Controls were not mentioned.  
Vague: Statement such as “appropriate positive and negative controls were included.”  
Identical: Controls identical to study samples were described.  
Other: Controls were dissimilar or partially similar (i.e., tissue control with smears or tissue control with cell block and ThinPrep samples run), or samples were too scant to include controls.

*> 70 % of publications based on IHC do not describe controls used to verify data and conclusions....*

# IHC controls to guide reliability of data...

**PAX8 expression in breast cancer – true or false...?**

Central for subtyping of unknown primary carcinoma; Ovary, uterine, kidney...

But...

Can PAX8 expression be seen in breast carcinoma??

Right choice, right use and results reported in positive and negative IHC control tissues needed to verify data

# IHC controls to guide reliability of data...

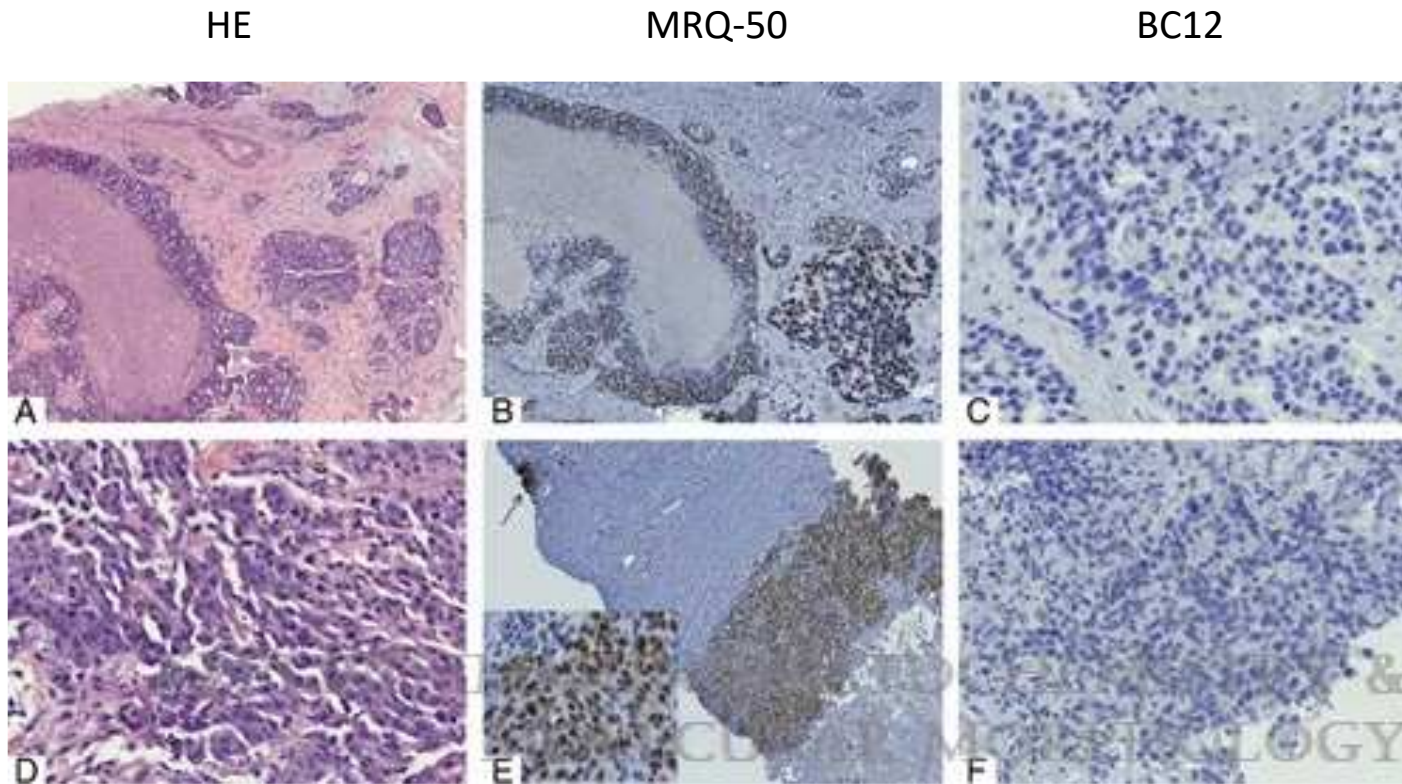


FIGURE 1

## Aberrant Immunostaining of Breast Carcinoma by MRQ-50 PAX8 Antibody

Singh, Kamaljeet; Hansen, Katrine; Quddus, M. Ruhul

Applied Immunohistochemistry & Molecular Morphology 28(4):e37-e38, April 2020.

doi: 10.1097/PAI.0000000000000682


Photomicrographs from 2 breast carcinomas with aberrant PAX8 expression by MRQ-50 clone. On staining with hematoxylin and eosin (A, D) both tumors were high grade with necrosis. Immunohistochemistry for PAX8 with MRQ-50 antibody (B, E) showed nuclear positivity in tumor cells and lymphocytes (arrow). PAX8 IHC with BC12 clone (C, F) did not stain tumor or lymphocytes.




# IHC controls to guide reliability of data...

NordiQC Assessments of PAX8 Immunoassays  
 Rasmus Roge, MD,\*† Ole Nielsen, HT,‡ Michael Bzorek, HT,§ Soren Nielsen, HT,\*  
 and Mogens Vyberg, MD\*†


Positive tissue control 1  
 Fallopian tuba

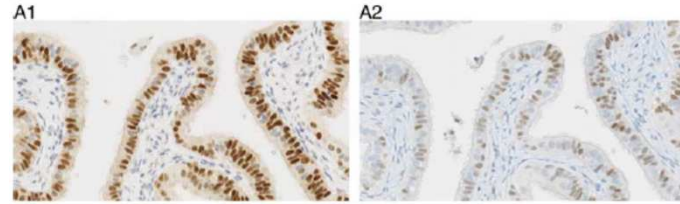


Positive tissue control 2  
 Kidney

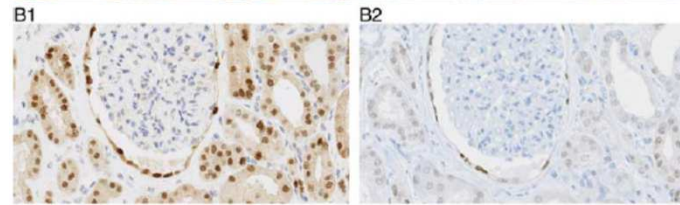


Tumour type 1  
 Ovarian carc.

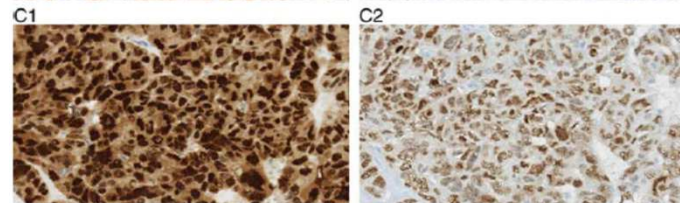


Tumour type 2  
 Renal cell carc.

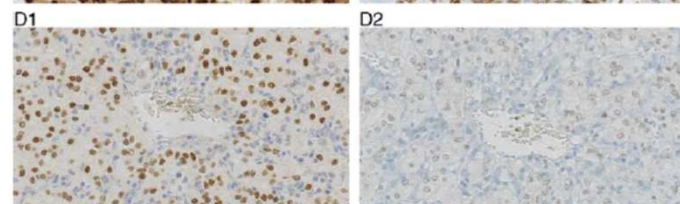

Negative tissue control 1  
 Tonsil

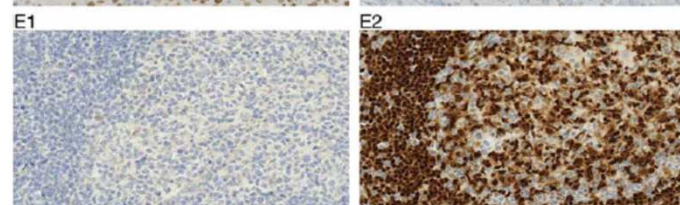

Level of analytical sensitivity

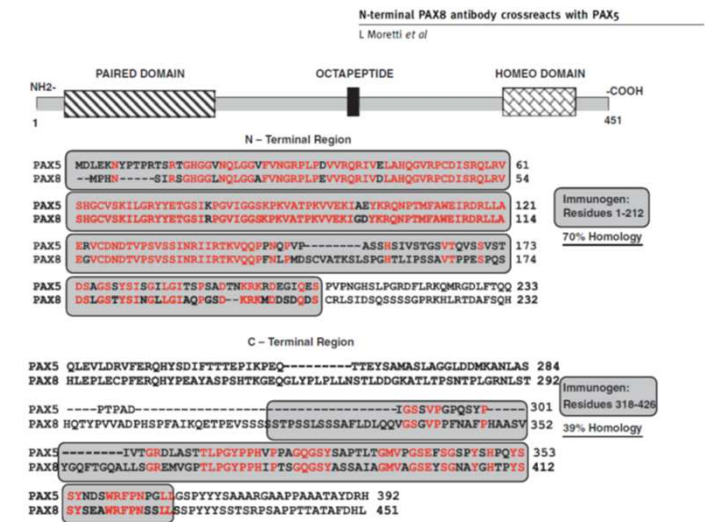


Level of analytical specificity

BC12 / SP348


MRQ-50 / pAb

# IHC controls to guide reliability of data...

MRQ-50  
(& pAb)

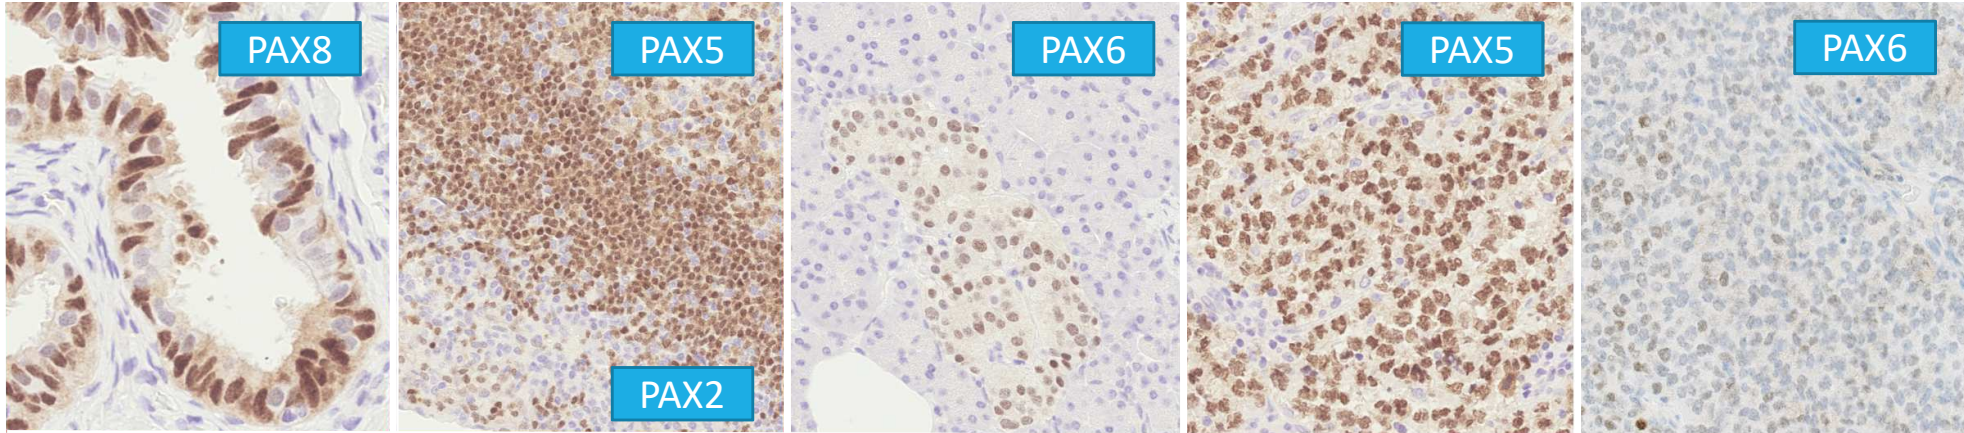

SP348  
(& BC12)

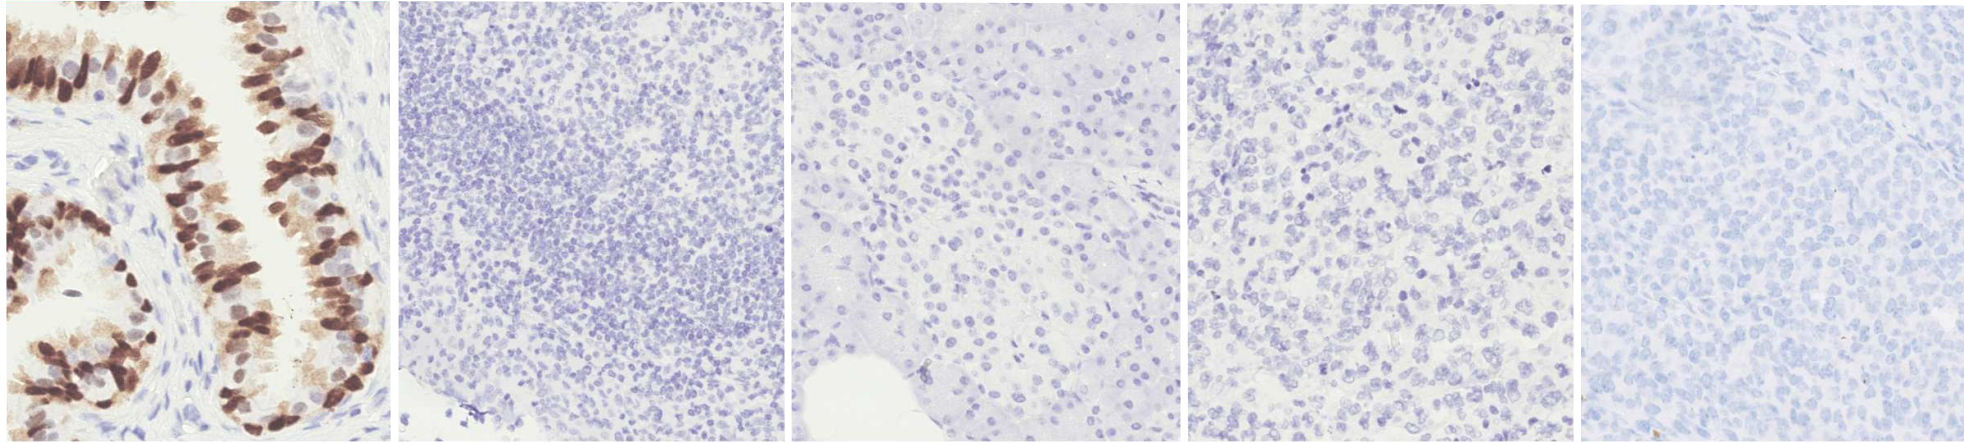

Fal. Tube

Tonsil

Pancreas

DLBCL


Breast carc.

# IHC controls to guide reliability of data...

## PAX8 expression in breast cancer – true or false...?


### Comparison of PAX8 Expression in Breast Carcinoma Using MRQ50 and BC12 Monoclonal Antibodies

*Kamaljeet Singh, MD, Linda C. Hanley, MD, C. James Sung, MD, and M. Rubel Qadus, MD, MPhil, Path*

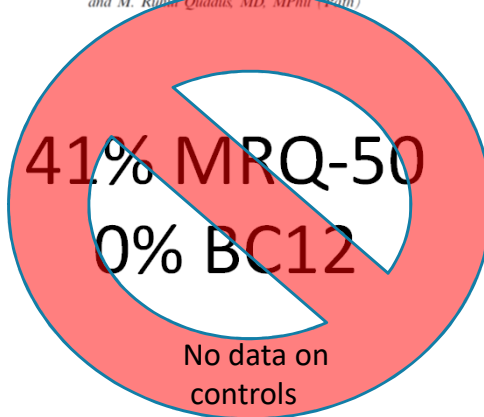


### Unexpected PAX8 Immunoreactivity in Metastatic High-grade Breast Cancer

*Mark R. Kilgore, MD, Dustin E. Bosch, MD, PhD, Kathi H. Adamson, MD, Paul E. Swanson, MD, Suzanne M. Dintzis, MD, PhD, and Maria H. Rendi, MD PhD*

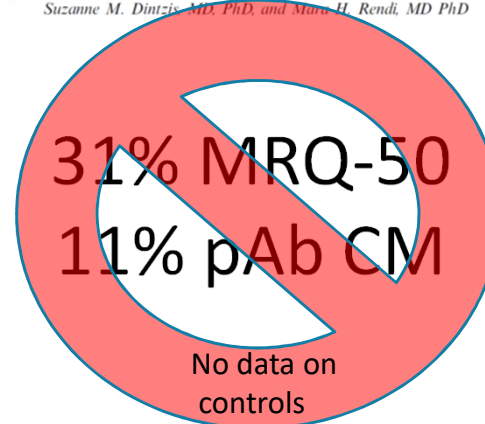

### Metastatic Carcinoma of Unknown Primary: Diagnostic Approach Using Immunohistochemistry



*James R. Conner, MD, PhD and Jason L. Hornick, MD, PhD*

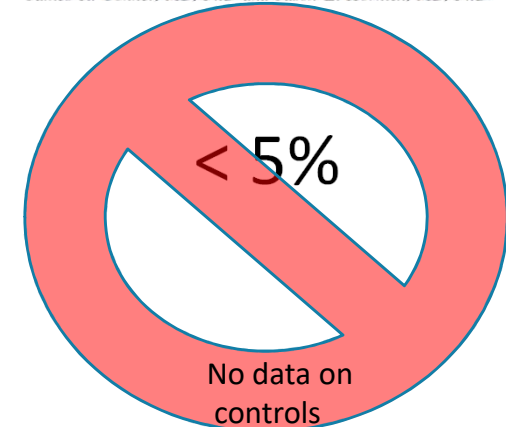


Right choice, right use and results reported in positive and negative IHC control tissues needed to verify data

# NordiQC data – PAX8


Graph 1. Proportion of sufficient results for PAX8 in the eight NordiQC runs performed

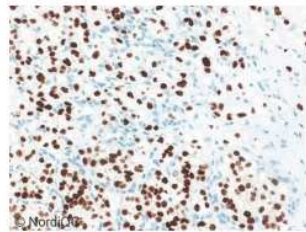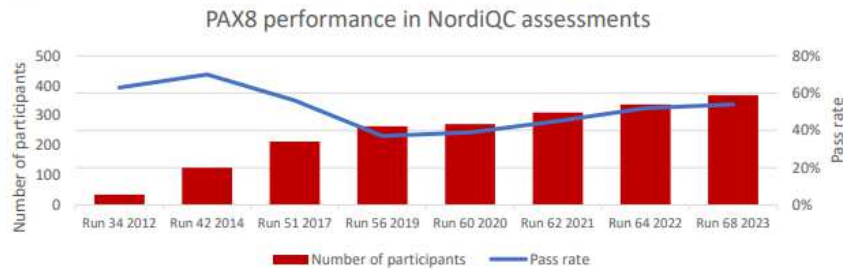


© NordiQC  
Fig. 4a x200  
Optimal PAX8 staining of the RCC using the same protocol as in Figs. 1a-3a. Virtually all the neoplastic cells show a moderate to strong nuclear staining reaction. No background staining is seen. Compare with Fig. 4b.

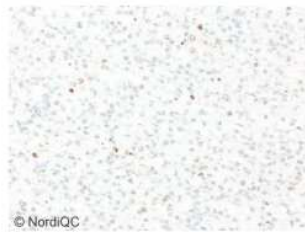

© NordiQC  
Fig. 4b x200  
Insufficient PAX8 staining of the RCC using the same protocol as in Figs. 1b-3b. Only a faint nuclear staining is seen in the vast majority of neoplastic cells. Compare with Fig. 4a.

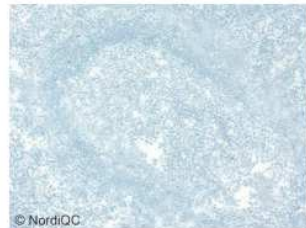

© NordiQC  
Fig. 5a x100  
PAX8 staining without PAX5 cross reactivity. PAX8 staining in tonsil using the same protocol as in Figs. 1a-4a. The mAb clone SP348 do not cross-react with PAX5, leaving the B-cells unstained. Compare with Fig. 5b.

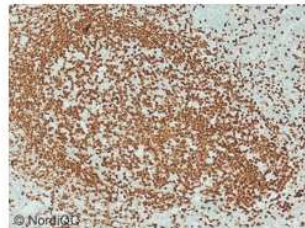

© NordiQC  
Fig. 5b x100  
PAX8 staining with PAX5 cross reactivity. PAX8 staining in tonsil using the same protocol as in Figs. 1b-4b. The mAb clone MRQ-50 cross-reacts with PAX5 resulting in nuclear staining reaction in virtually all B-cells. Compare with Fig. 5a.

Table 1. Antibodies and assessment marks for PAX8, run 68

Concentrated antibodies	n	Vendor	Optimal	Good	Borderline	Poor	Suff. <sup>1</sup>	OR <sup>2</sup>
mAb clone <b>BC12*</b>	9	Biocare Zytomed Systems	-	3	7	3	23%	-
mAb clone <b>MRQ-50</b>	16	Cell Marque	-	8	6	2	50%	-
mAb clone <b>PAX8R1</b>	1	Abcam	-	-	1	-	-	-
mAb clone <b>ZM28</b>	1	Zeta Corporation	-	1	-	-	-	-
rmAb clone <b>EP298<sup>5*</sup></b>	1	Epitomics <sup>5</sup>	-	1	-	-	-	-
rmAb clone <b>EP331*</b>	10	Cell Marque	-	5	8	1	36%	-
rmAb clone <b>EP331*</b>	4	Epitomics	-	5	8	1	36%	-
rmAb clone <b>SP348*</b>	146	Abcam Genova Spring Bioscience	102	31	9	4	91%	70%
rmAb clone <b>ZR-1*</b>	2	Zeta Corporation BioSite	1	-	2	1	-	-
rmAb clone <b>BP6157*</b>	2	Biolynx	-	1	1	-	-	-
rmAb clone <b>QR016*</b>	7	Quartett	3	3	1	-	86%	43%
pAb, <b>10336-1-AP</b>	11	Proteintech	-	1	3	7	9%	-
pAb, <b>363A-15</b>	1	Cell Marque	-	-	1	-	-	-
pAb, <b>CP379 AK</b>	3	Biocare	-	-	1	2	-	-
pAb, <b>RBK047</b>	3	Zytomed Systems Diagomics	-	-	3	-	-	-
<b>Conc total</b>	<b>223</b>		<b>106</b>	<b>54</b>	<b>43</b>	<b>20</b>	<b>72%</b>	<b>48%</b>
<b>Ready-To-Use antibodies</b>								
mAb clone <b>MRQ-50, 760-4618 (VRPS)<sup>3</sup></b>	6	Ventana/Roche	-	-	-	6	0%	0%
mAb clone <b>MRQ-50, 760-4618 (LMPS)<sup>4</sup></b>	49	Ventana/Roche	-	3	34	12	6%	0%
rmAb clone, <b>EP331* 760-6077 (VRPS)<sup>3</sup></b>	3	Ventana/Cell Marque	-	1	2	-	-	-
rmAb clone, <b>EP331* 760-6077 (LMPS)<sup>4</sup></b>	11	Ventana/Cell Marque	-	4	6	1	36%	0%
mAb clone, <b>BC12* API438</b>	6	Biocare Medical	-	2	4	-	33%	0%
mAb clone <b>IHC008 P1177R06</b>	3	DCS	-	-	3	-	-	-
rmAb clone <b>ZR-1* Z2202</b>	2	Zeta corporation	-	-	1	1	-	-
rmAb clone <b>SP348* M6481</b>	3	Spring Bioscience	2	1	-	-	-	-
rmAb clone <b>2774R ANB31</b>	1	Biogenex	-	-	1	-	-	-
rmAb clone <b>GR002* GT210202</b>	1	GeneTech	1	-	-	-	-	-
rmAb clone <b>QR016* P-P008</b>	2	Quartett	1	1	-	-	-	-
rmAb clone <b>EP331* 363M/AC0338</b>	12	Cell Marque	-	3	7	2	25%	0%
rmAb clone <b>SP348* 363R-38</b>	4	Cell Marque	2	1	1	-	-	-
mAb clone <b>MRQ-50, 363M-10/17/18 363A17/18</b>	24	Cell Marque	-	5	13	6	21%	0%
pAb clone <b>363A-17/18 363A17/18</b>	4	Cell Marque	-	-	3	1	-	-
mAb clone <b>MRQ-50, MAD-000550QD</b>	6	Master Diagnostica	-	4	1	1	67%	0%
rmAb clone <b>RM436* 8257-C010</b>	2	Sakura Finetek	1	1	-	-	-	-
rmAb clone <b>IHC048*</b>	1	GenomeMe	-	-	1	-	-	-
mAb clone <b>C12A32</b>	1	Celnovte	-	1	-	-	-	-
Clone <b>MXR013* RMA-1024</b>	2	Fuzhou Maixin	2	-	-	-	-	-
Clone <b>H5A8 DTBL0220101</b>	1	DaTe Bioengineering Technology	1	-	-	-	-	-
Unknown	1		-	-	-	1	-	-
<b>RTU total</b>	<b>145</b>		<b>10</b>	<b>27</b>	<b>77</b>	<b>31</b>	<b>26%</b>	<b>8%</b>
<b>Total</b>	<b>368</b>		<b>116</b>	<b>81</b>	<b>120</b>	<b>51</b>	<b>54%</b>	
<b>Proportion</b>			<b>32%</b>	<b>22%</b>	<b>32%</b>	<b>14%</b>	<b>54%</b>	

1) Proportion of sufficient stains (optimal or good). (≥5 assessed protocols).

2) Proportion of Optimal Results (≥5 assessed protocols).

3) Vendor Recommended Protocol Settings (VRPS) to a specific RTU product applied on the vendor recommended platform(s) (≥5 assessed protocols).

4) Laboratory Modified Protocol Settings (LMPS) to a specific RTU product (≥5 assessed protocols).

5) Ab terminated by vendor.

\*Clones that do not show cross reactivity with PAX5.

# References central for the area of IHC controls

The "Kick-off" phase for

"Standardization of IHC controls"

Definitions and requirements

Usage

Potentials / Limitations

Perspectives

## REVIEW ARTICLE

*Appl Immunohistochem Mol Morphol* . Volume 22, Number 4, October 2014

### Standardization of Negative Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Panel

*Emina E. Torlakovic, MD, PhD,\*†‡ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),§¶  
John Garratt, RT,†‡## Blake Gilks, MD, FRCPC,†‡\*\* Elizabeth Hyjek, MD, PhD,\*  
Merdol Ibrahim, PhD,†† Rodney Miller, MD,‡‡ Soren Nielsen, HT, CT,§§||  
Eugen B. Petcu, MD, PhD,§ Paul E. Swanson, MD,¶¶ Clive R. Taylor, MD, PhD,##  
and Mogens Vyberg, MD§§||*

## REVIEW ARTICLE


*Appl Immunohistochem Mol Morphol* • Volume 23, Number 1, January 2015

### Standardization of Positive Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Committee

*Emina E. Torlakovic, MD, PhD,\*† Soren Nielsen, HT, CT,‡§ Glenn Francis, MBBS, FRCPA,  
MBA, FFSc (RCPA),||¶## John Garratt, RT,†\*\* Blake Gilks, MD, FRCPC,†††  
Jeffrey D. Goldsmith, MD,‡‡ Jason L. Hornick, MD, PhD,\*§§ Elizabeth Hyjek, MD, PhD,\*  
Merdol Ibrahim, PhD,|| Keith Miller, FIBMS,|| Eugen Petcu, MD, PhD,||  
Paul E. Swanson, MD,¶¶## Xiaoge Zhou, MD,\*\*\*††† Clive R. Taylor, MD, PhD,‡‡‡  
and Mogens Vyberg, MD‡§*


# Tissue controls

- Reagent and **tissue** controls are necessary for the validation/verification of immunohistochemical staining results.
- Tissue controls are the most valuable tool to monitor the specificity and sensitivity for IHC
  - Internal positive and negative tissue control
    - Cells/structures within the patient material
  - External positive and negative tissue control
    - Slide next to patient material – **on-slide optimally**

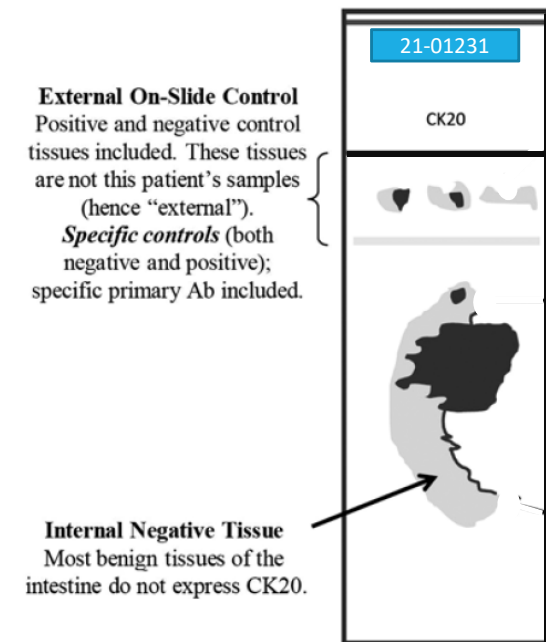


# How to use internal tissue controls

**TABLE 2. Examples of IHC Assays Where Preferential Use of Internal Positive Controls Recommended**

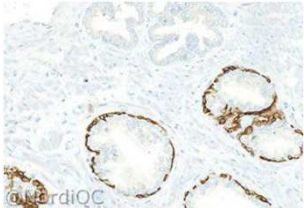IHC Assay	Use	Comments
Cytokeratin 5 	Demonstration of basal cells in glandular structures of prostate to differentiate between benign (positive) and malignant (negative) glands	Interpretation of the results in the tumor directly depends on clear demonstration of internal positive control  Tested sample may be completely negative if no normal tissue is present
Mismatch repair proteins (MLH1, MSH2, PMS2, MSH6)	Absence of expression in the cells of colon or endometrial adenocarcinoma is abnormal; patients referred for molecular testing to rule out Lynch Syndrome	Interpretation of the results in the tumor directly depends on clear demonstration of internal positive control



Internal positive tissue controls; Principally ideal as processed identically to patient relevant material / target evaluated

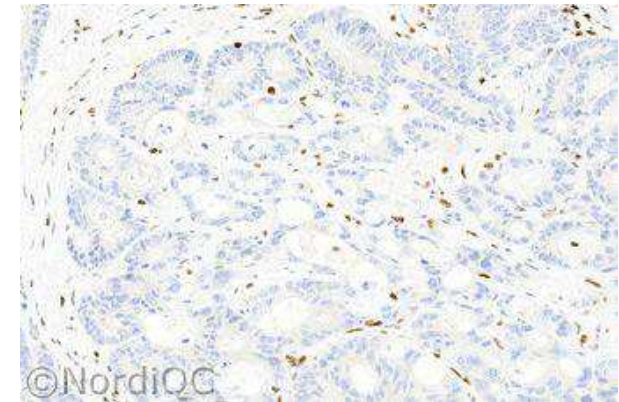

If internal positive control is neg or dubious – test is repeated.

Target analyte	Application	Internal control to confirm "true" loss
BAP1, MTAP	Mesothelioma	Stromal cells
p53	Gynological carc.	Stromal cells
PTEN	Lung and gynecological carc.	Stromal and benign cells
MMR (MLH1, MSH2, MSH6, PMS2)	Lynch syndrome	Stromal cells / lymphocytes
SMAD4	Pancreas and GI carc.	Stromal and benign cells

# Limitations of internal tissue controls

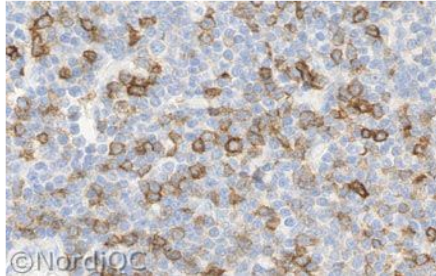
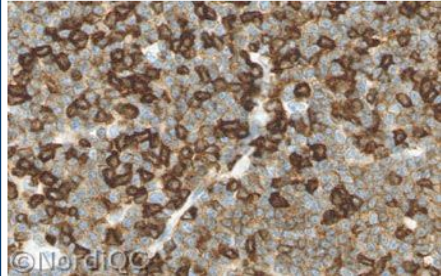


Fig. 4a. Optimal staining for CD5 of the B-CLL no. 5 using same protocol as in Figs. 1a - 4a. The majority of the neoplastic cells show a moderate and distinct staining reaction, while the infiltrating normal T-cells show a strong staining reaction.

Fig. 4b. Insufficient staining for CD5 of the B-CLL using same protocol as in Figs. 1b - 3b - same field as in Fig. 4a. The neoplastic cells are virtually negative and only the normal T-cells are clearly demonstrated.

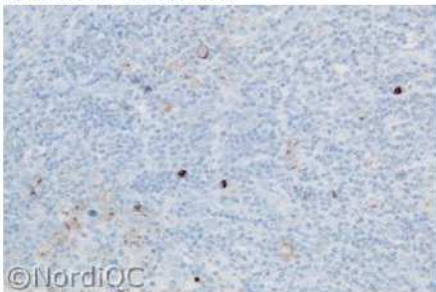
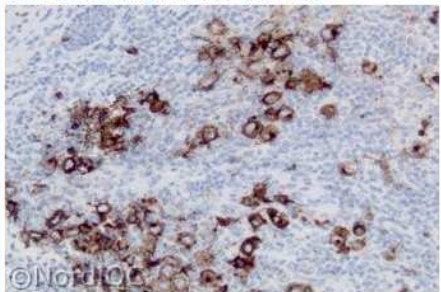


Fig. 2a. Optimal CD15 staining of the Hodgkin lymphoma no 2 (NS) using same protocol as in Fig. 1a. The Reed-Sternberg and Hodgkin cells show a strong membranous staining and a dot-like positivity.

Fig. 2b. CD15 staining of the Hodgkin lymphoma no 2 (NS) using same protocol as in Fig. 1b. Only few Reed-Sternberg and Hodgkin cells show a weak staining - same field as in Fig. 2a.

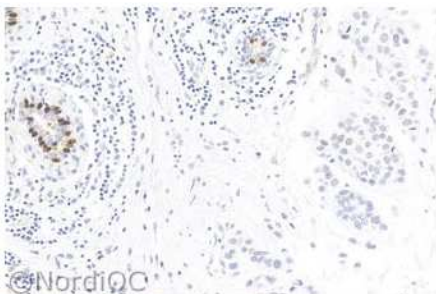
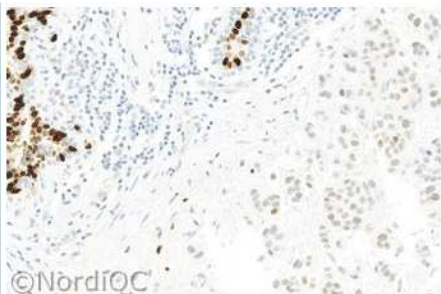


Fig. 3a. Optimal ER staining of the breast ductal carcinoma no. 3 with 60 - 80 % cells positive. A weak but distinct nuclear staining is seen in the appropriate proportion of the neoplastic cells. Same protocol as in Figs. 1a and 2a.


Fig. 3b. Insufficient ER staining of the breast ductal carcinoma no. 3 with 60 - 80 % cells positive using same protocol as in Figs. 1b and 2b - same field as in Fig. 3a. Only dispersed neoplastic cells show an equivocal staining

Internal positive tissue controls;

In general not applicable as positive controls due to levels of expression may not be relevant for level of test calibration

e.g. CD5, CD15, CD34, CD45, CD56, S100, ER, PD-L1 etc

CD5;  
Tonsil  
Mantle zone  
  
Critical  
control

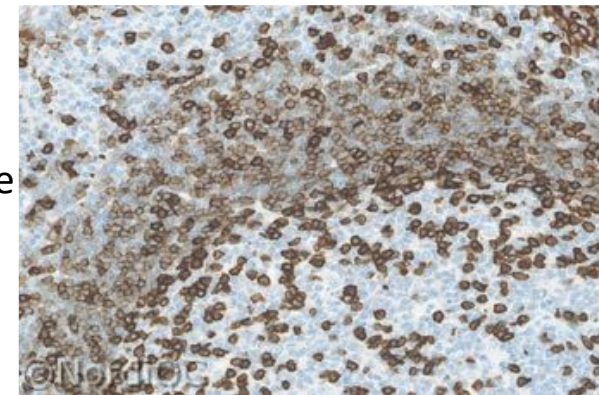



# Critical tissue controls = ICAPCs

## IHC Critical Assay Performance Controls (ICAPCs)

are basically human positive control tissues with

- clinical relevant range of target analyte (antigen) – especially with low limit detection
- well characterized expression pattern – preferable normal tissues
- predictable levels and specified cellular and architectural localization

	High expression	Low expression	No expression
Purpose	Right antibody	Right analytical sensitivity	Basic right specificity


REVIEW ARTICLE

*Appl Immunohistochem Mol Morphol* • Volume 23, Number 1, January 2015

**Standardization of Positive Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Committee**

*Emina E. Torlakovic, MD, PhD,\*† Soren Nielsen, HT, CT,‡§ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),||\*## John Garratt, RT,†\*\* Blake Gilks, MD, FRCPC,††† Jeffrey D. Goldsmith, MD,‡‡‡ Jason L. Hornick, MD, PhD,\*§§ Elizabeth Hyjek, MD, PhD,\* Merdol Ibrahim, PhD,||| Keith Miller, FIBMS,||| Eugen Petcu, MD, PhD,|| Paul E. Swanson, MD,\*## Xiaoge Zhou, MD,\*\*\*††† Clive R. Taylor, MD, PhD,‡‡‡ and Mogens Vyberg, MD‡§*

CD5;  
Tonsil  
Mantle zone  
  
Critical  
control

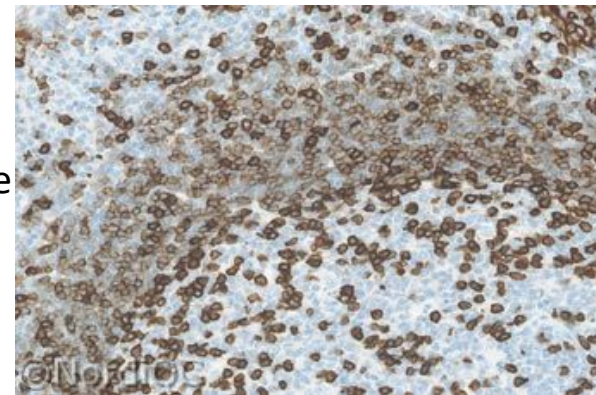

# Test Performance Characteristics - TPCs

Test performance characteristics;

Which staining pattern characterizes an optimally calibrated IHC assay for a specific purpose?

Analytical sensitivity

Analytical specificity

Precision / reproducibility of IHC assay


Which tissues / cellular structures show the clinical relevant range of the target analyte with focus on required low level of demonstration – **CRITICAL CONTROLS - ICAPCs?**

# Fit For Purpose; the selection....

CD56

CD45

Colon

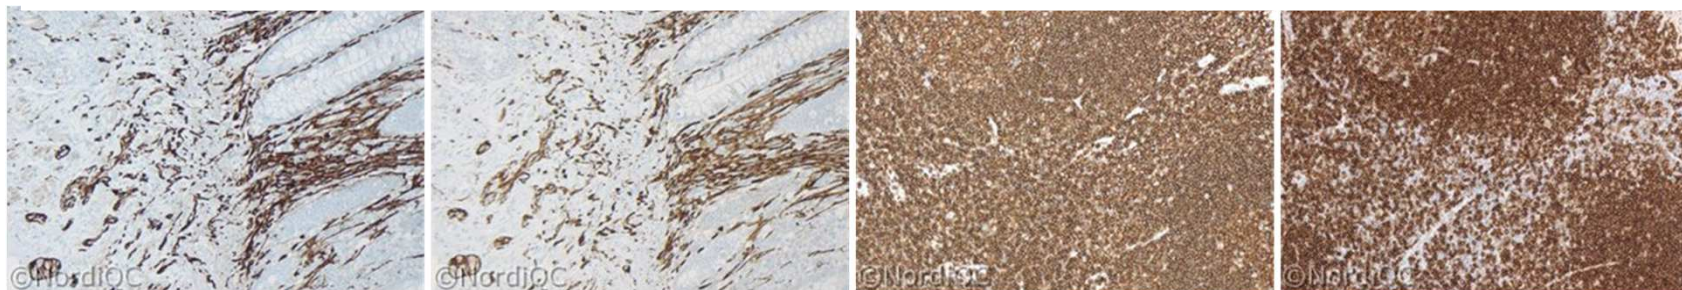

Tonsil

Test A

Test B

Test A


Test B

# Fit For Purpose; the selection....

CD56


CD45

Colon

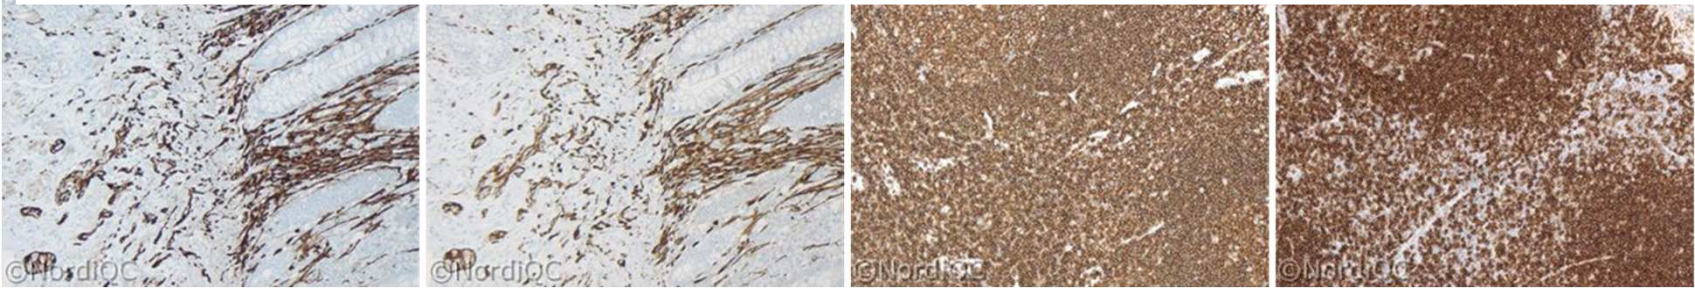

Tonsil

NET

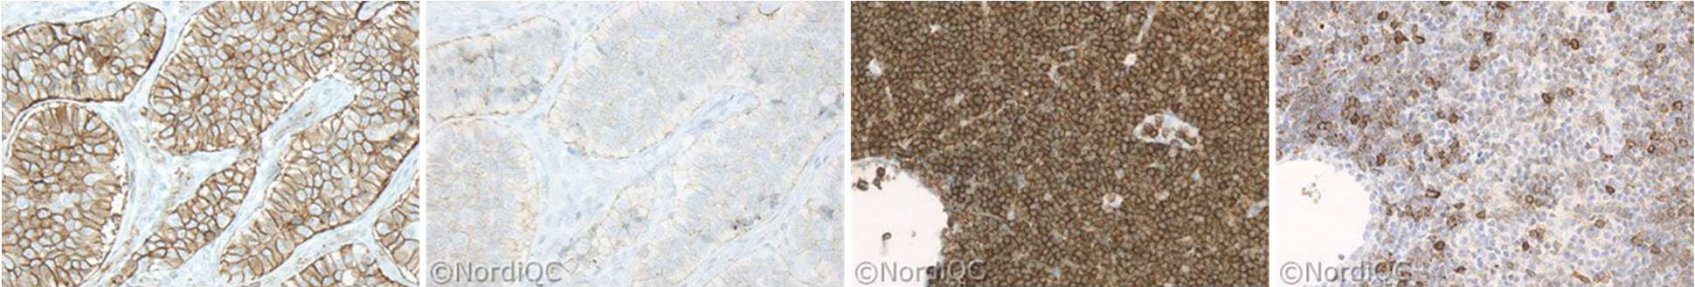

B-CLL

Test A

Test B

Test A


Test B

# Fit For Purpose; the selection....

CD56


CD45

Colon

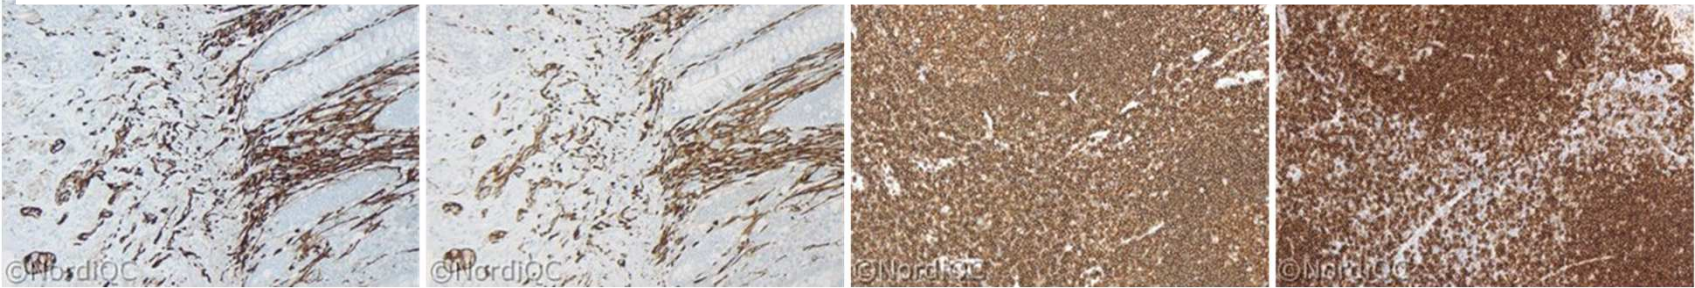


Tonsil

NET

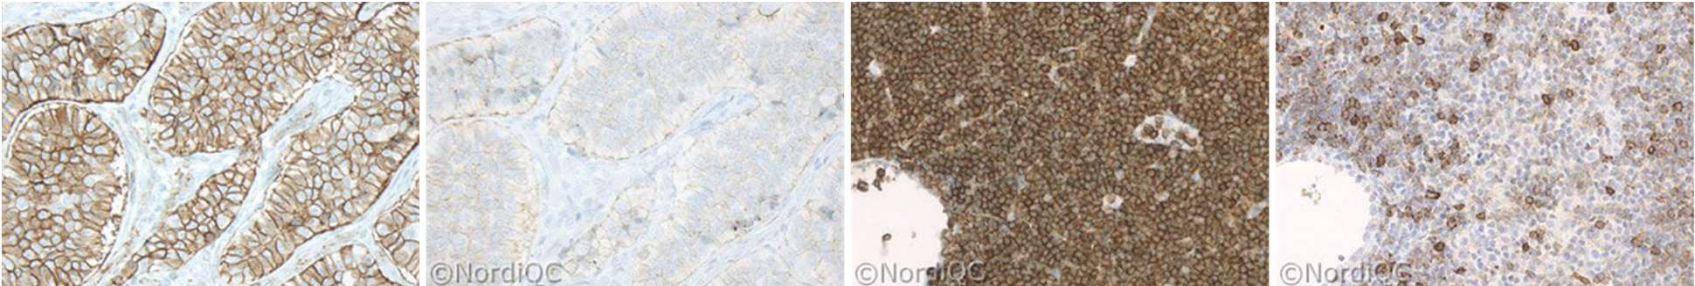

B-CLL

Tonsil

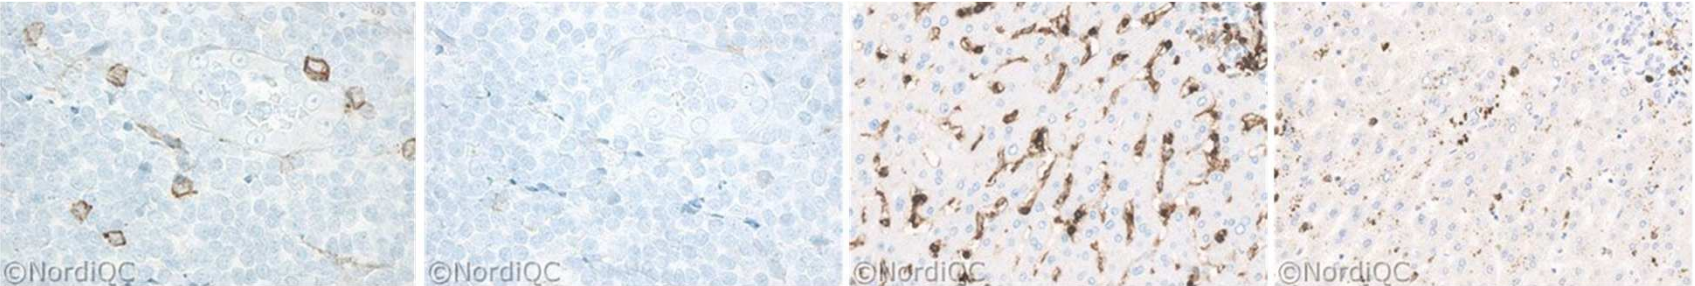

Liver


Test A

Test B


Test A

Test B

# Fit For Purpose; the selection....

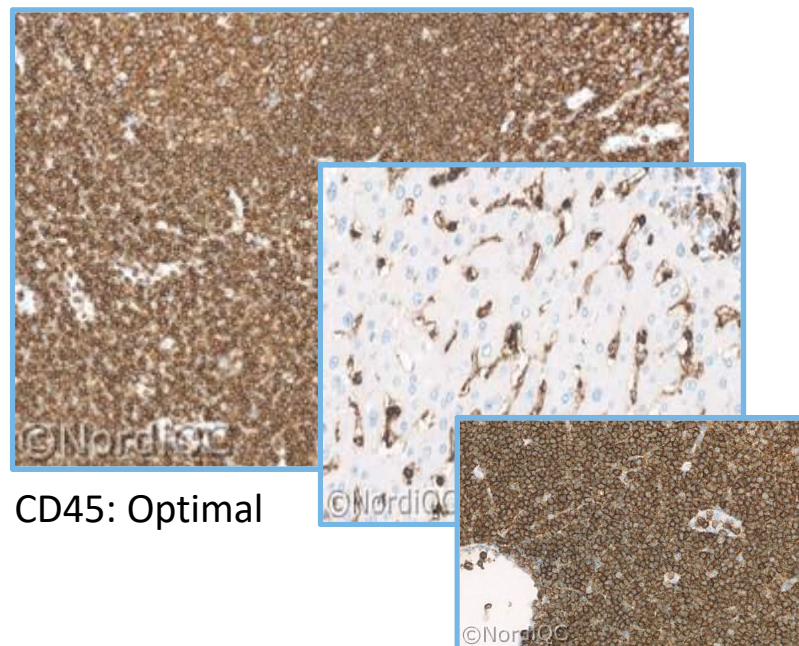

CD45: Optimal

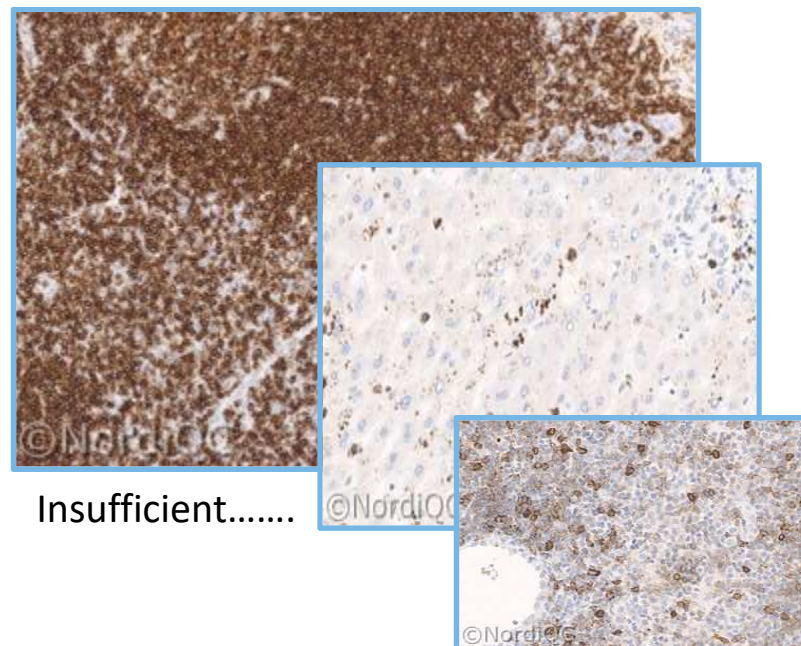

Insufficient.....

Tissues/cells with only high expression will not identify:

1. A poorly calibrated IHC assay
2. A reduced sensitivity in an optimally calibrated IHC assay

If an IHC test is used to identify the target antigen being expressed at different levels, controls must reflect this!

# iCAPCs - concept

IHC Critical Assay Performance Controls (iCAPCs)

Which tissues are recommended ?

What is the expected staining pattern ?

Which tissues / cells are critical ?

Right antibody

Appropriate level of sensitivity

Guidance level of specificity

REVIEW ARTICLE

*Appl Immunohistochem Mol Morphol* • Volume 23, Number 1, January 2015

**Standardization of Positive Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Committee**


*Emina E. Torlakovic, MD, PhD,\*† Soren Nielsen, HT, CT,‡§ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),||¶# John Garratt, RT,†\*\* Blake Gilks, MD, FRCPC,††† Jeffrey D. Goldsmith, MD,‡‡ Jason L. Hornick, MD, PhD,\*§§ Elizabeth Hyjek, MD, PhD,\* Merdol Ibrahim, PhD,|| Keith Miller, FIBMS,|| Eugen Petcu, MD, PhD,|| Paul E. Swanson, MD,¶## Xiaoge Zhou, MD,\*\*\*††† Clive R. Taylor, MD, PhD,‡‡‡ and Mogens Vyberg, MD‡§*

ASCO special articles

**Estrogen and Progesterone Receptor Testing in Breast Cancer: ASCO/CAP Guideline Update**

Kimberly H. Allison, MD<sup>1</sup>; M. Elizabeth H. Hammond, MD<sup>2</sup>; Mitchell Dowsett, PhD<sup>3</sup>; Shannon E. McKernin<sup>4</sup>; Lisa A. Carey, MD<sup>5</sup>; Patrick L. Fitzgibbons, MD<sup>6</sup>; Daniel F. Hayes, MD<sup>7</sup>; Sunil R. Lakhani, MD<sup>8,9</sup>; Mariana Chavez-MacGregor, MSc<sup>10</sup>; Jane Perlmutter, PhD<sup>11</sup>; Charles M. Perou, PhD<sup>12</sup>; Meredith M. Regan, ScD<sup>12</sup>; David L. Rimm, MD, PhD<sup>13</sup>; W. Fraser Symmans, MD<sup>10</sup>; Emina E. Torlakovic, MD, PhD<sup>14,15</sup>; Leticia Varella, MD<sup>16</sup>; Giuseppe Viale, MD<sup>17,18</sup>; Tracey F. Weisberg, MD<sup>19</sup>; Lisa M. McShane, PhD<sup>20</sup>; and Antonio C. Wolff, MD<sup>21</sup>

J Clin Oncol 38:1346-1366. © 2020 by American Society of Clinical Oncology

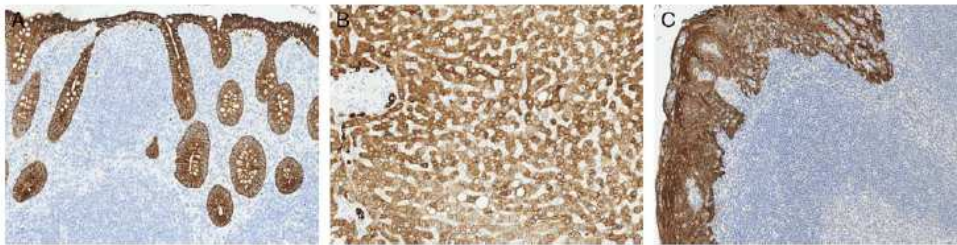

**FIGURE 1.** Pan-keratin iCAPC. A, Appendix: virtually all columnar epithelial cells must show a moderate to strong predominantly cytoplasmic staining reaction (a membranous accentuation will typically be seen). B, Liver: the vast majority of hepatocytes must show at least weak to moderate cytoplasmic staining reaction with a membranous accentuation (LLOD). C, Tonsil: all squamous epithelial cells must show a moderate to strong cytoplasmic staining reaction. Cytokeratin (CK)-positive interstitial reticulum cells (CIRCs) with dendritic/reticular pattern can show a weak to moderate cytoplasmic staining reaction (LLOD). iCAPC indicates immunohistochemistry critical assay performance controls; LLOD, low limit of detection.

Examples for 17 markers

General expected patterns

High expression  
(Right antibody)


Low expression  
(Appropriate sensitivity)

No expression  
(Appropriate specificity)

**Which tissue**  
**Which cells**  
**Which extension**  
**Which intensity**



**FIGURE 7.** TTF-1 iCAPC. A, Thyroid: virtually all epithelial cells must show a strong nuclear staining reaction. B, Lung: virtually all pneumocytes and basal cells of terminal bronchi must show a moderate to strong nuclear staining reaction. Columnar epithelial cells of terminal bronchi must show an at least weak nuclear staining reaction (LLOD). C, Tonsil: no staining reaction must be seen. iCAPC indicates immunohistochemistry critical assay performance controls; LLOD, low limit of detection.

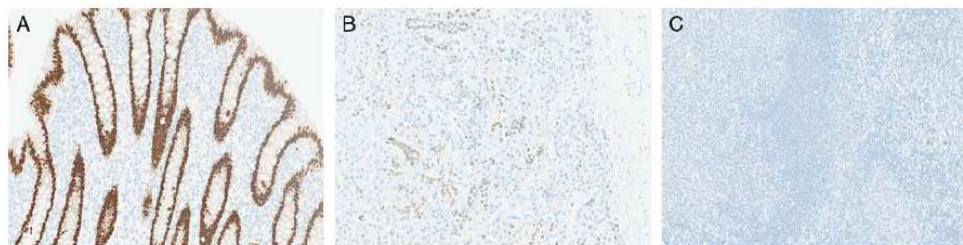

**FIGURE 8.** CDX-2 iCAPC. A, Appendix: virtually all epithelial cells must show a strong nuclear staining reaction. A weak cytoplasmic staining reaction in addition to strong nuclear staining is often present. B, Pancreas: the majority of epithelial cells of intercalated ducts must show a weak to moderate nuclear staining reaction (LLOD). C, Tonsil: no staining reaction must be seen. iCAPC indicates immunohistochemistry critical assay performance controls; LLOD, low limit of detection.



# NordiQC IHC tissue control atlas – open from 05.2022



## Recommended controls

Search:

Epitope ▲	Tissues ⚡	Actions ⚡
ALK (lung)	Appendix/colon, Tonsil	<a href="#">See controls</a>
AMACR	Kidney, Prostate	<a href="#">See controls</a>
ASMA	Appendix/colon, Liver	<a href="#">See controls</a>
Bcl-2	Tonsil	<a href="#">See controls</a>
Bcl-6	Tonsil	<a href="#">See controls</a>
BSAP	Hodgkin lymphoma, Tonsil	<a href="#">See controls</a>
C-MYC	Appendix/colon, Tonsil	<a href="#">See controls</a>
CD3	Appendix/colon, Tonsil	<a href="#">See controls</a>
CD4	Liver, Tonsil	<a href="#">See controls</a>
CD5	Tonsil	<a href="#">See controls</a>
CD8	Appendix/colon, Tonsil	<a href="#">See controls</a>
CD10	Kidney, Tonsil	<a href="#">See controls</a>
CD15	Kidney, Tonsil	<a href="#">See controls</a>
CD19	Appendix/colon, Tonsil	<a href="#">See controls</a>
CD20	Appendix/colon, Tonsil	<a href="#">See controls</a>
CD23	Tonsil	<a href="#">See controls</a>
CD30	Tonsil	<a href="#">See controls</a>
CD31	Appendix/colon, Liver, Tonsil	<a href="#">See controls</a>

Available for NordiQC participants

Tissues

Purpose

Reaction patterns




Online scans accessible

# NordiQC IHC tissue control atlas – open from 05.2022



Info ▾ Modules ▾ Assessments Protocols Controls Events ▾ [SN](#)

## CDX2 - CDX2

Control type	Positive tissue control High expression level	Positive tissue control Low expression levels	Negative tissue control
Tissue	Appendix/colon	Pancreas	Tonsil
Description	<p>All epithelial cells must show a strong nuclear staining reaction.</p> <p><i>Note, a weak cytoplasmic staining reaction in CDX2 positive cells can be seen and should be accepted if signal-to-noise ratio otherwise is acceptable.</i></p>	<p>The vast majority of epithelial cells of intercalated ducts must show a weak to moderate nuclear staining reaction.</p>	<p>No staining reaction should be seen.</p> <p><i>Note, dispersed lymphocytes can show a faint nuclear staining reaction.</i></p>
Example	 <p>Click to enlarge</p>	 <p>Click to enlarge</p>	 <p>Click to enlarge</p>

Back

Available for NordiQC participants


Tissues

Purpose

Reaction patterns

Online scans accessible

## NordiQC IHC tissue control atlas – open from 05.2022

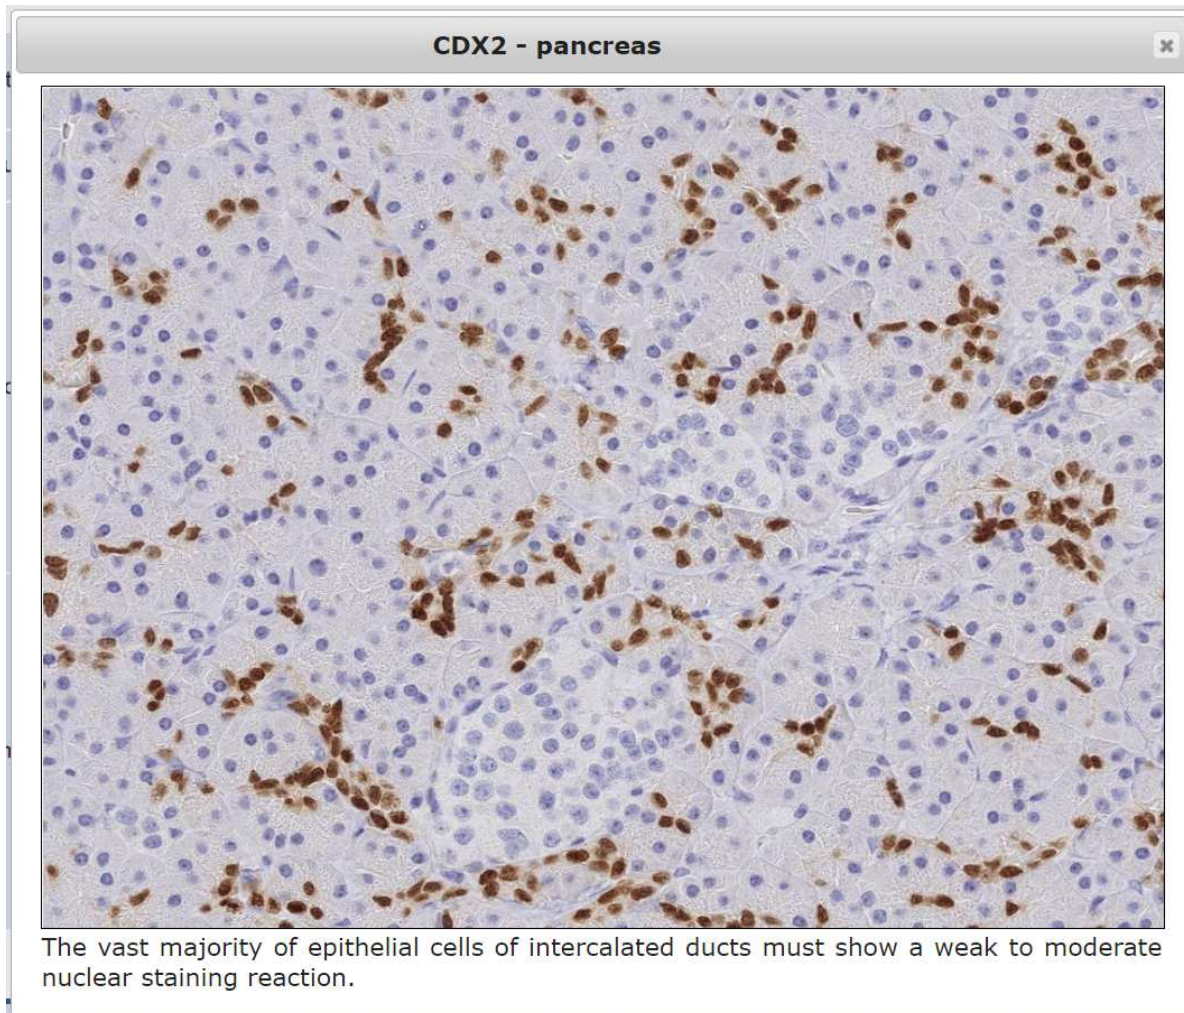

Available for NordiQC participants

Tissues

Purpose

Reaction patterns

Online scans accessible

# Challenges for ICAPCs / Critical Controls

1. Limited access to relevant tissues – rare incidences
  - ALK (lung), ROS1, Myogenin..
2. New markers not described in details – no data on test performance characteristics
  - SATB2, Claudin-4, PRAME, TRPS1....
3. Limited access to reference material and/or critical expression levels
  - PD-L1, HER2, ER...



Where to start – how to end.....

# Role of cell lines & histoids for IHC test development

1. Limited access to relevant tissues – rare incidences
  - ALK (lung), ROS1, Myogenin..
3. Limited access to reference material and/or critical expression levels
  - PD-L1, HER2, ER...

Starting help to guide development – validation still required....

**HER2, ER, PGR Dynamic Range Analyte Control**  
Multi-purpose control material for same slide use to improve the quality and reliability of your assays

Welcome to HistoCyte Laboratories  
We manufacture a range of cell line controls for same slide use in immunohistochemistry (IHC) and in situ hybridization (ISH). HistoCyte Laboratories Ltd have developed unique processes that allow the production of high density cell preparations that retain their original morphology. Through careful selection of cell types we can generate a range of positive and negative controls to determine effective performance of reagents used in slide based assessments.

**Products**  
View our range of high quality, reliable control material

**Services**  
We offer a range of contract services to assist in product development

- Biomarker Characterization
- Proof of Concept
- Custom Cell Line Development
- Assay Design
- QMS Auditing

**About**  
Learn more about our company and history

[www.histocyte.com](http://www.histocyte.com)

Cell lines

ALK and ROS1 being +/-

HER2, ER, PR and PD-L1 with dynamic range

**Specimen collection all the way through advanced diagnostics.**  
Quality products to empower your complete lab workflow are now available for ordering on a single site, delivered with the customer service you've come to know and love.

**Advanced Diagnostics**  
IHC reagents deliver high quality staining with superior results

**Stains**  
American Master/Tech and StatLab stains and kits to meet your needs

**Coverslips and Slides**  
High-quality slides and accessories to meet a wide variety of preferences

**All Products**  
Search all categories of products to support your complete lab workflow



[www.statlab.com](http://www.statlab.com)

Histoids / Faux tissue

ALK +/-

HER2, PD-L1 with dynamic range

# Histoids / Faux tissue – TruQ IHC controls

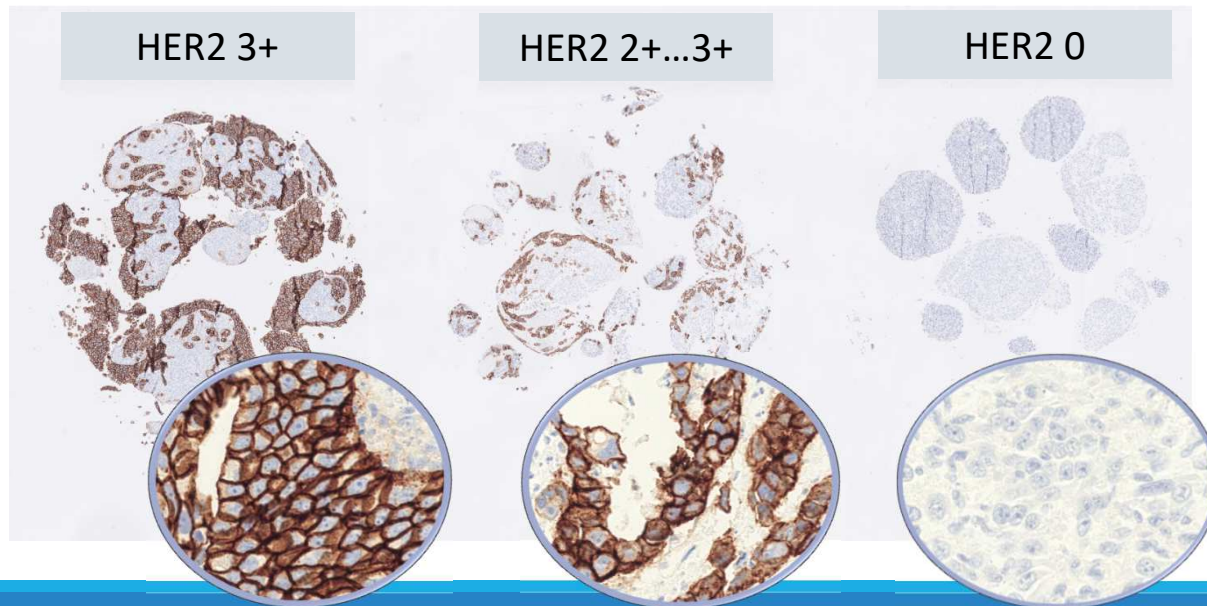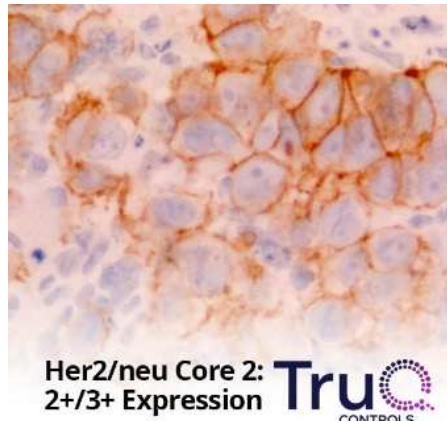

Tissue core with IHC 3+ and IHC 2+ almost identical concerning expression levels.

No IHC 1+ tissue

Design seems less adequate for "precision testing" for HER2 IHC both "classical" and HER2 low.

# Role of cell lines for IHC test development

## HER2 Analyte Control<sup>DR</sup>

Cell line controls for immunohistochemistry and in situ hybridization.

### Research Use Only

#### PRODUCT AVAILABILITY

Product Code	Product Description
HCL026	X2 Cut slides
HCL027	X5 Cut slides
HCL028	X1 Cell microarray block

#### APPLICATION

This product is suitable for use in immunohistochemistry and in situ hybridization.

#### MATERIALS

Four formalin fixed paraffin embedded cell lines with a dynamic range (DR) of expression for Human Epidermal growth factor Receptor 2 (HER2).

Cell line A: Breast adenocarcinoma  
 Cell line B: Breast adenocarcinoma  
 Cell line C: Gastric adenocarcinoma  
 Cell line D: Breast adenocarcinoma

Cells are fixed in 10% neutral buffered formalin and paraffin wax embedded. Sections are cut at 4µm, mounted on positively charged slides and baked overnight at 37°C.



Cell microarrays (CMA) contain cores that are 1.5-2mm in diameter and 3-3.5mm in length. It is possible to obtain over 300 sections depending on thickness.



### Expression Profile

Cell Line	IHC for HER2	FISH for HER2 gene amplification
A	0	Non-amplified
B	1+	Non-amplified
C	2+	Equivocal
D	3+	Amplified

### Storage and Handling

Store at 2-8°C. Do not freeze (for expiration date please see the product label)



### WARNINGS AND PRECAUTIONS

1. The product is intended for research use only.
2. It is the responsibility of the end user to determine suitability with their reagents and procedures within their laboratory.
3. Do not use after expiration date printed on product labels. The user must validate any storage conditions other than those specified in the package insert.

### TROUBLE SHOOTING

For further help please feel free to contact HistoCyte Laboratories Ltd at [info@histocyte.com](mailto:info@histocyte.com) or call +44 (0)191 603 1007.

 For updates and additional product information please visit: [www.HistoCyte.com](http://www.HistoCyte.com)

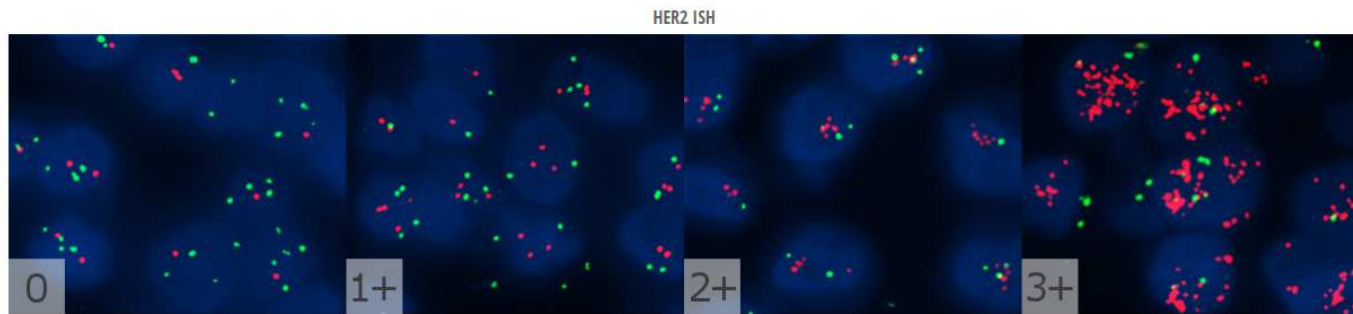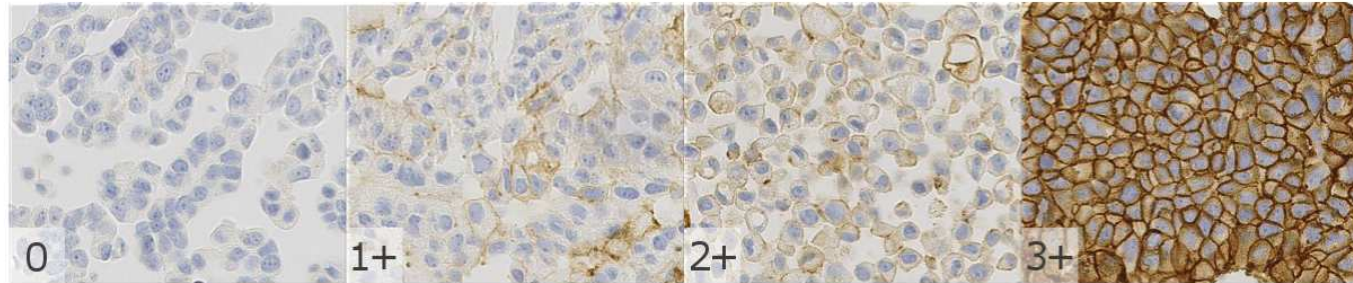


Still need evidence/proof (VALIDATION) how to correlate any change in staining pattern in cell lines for accuracy in tissues of breast carcinoma.

Tissue and cell line expression robustness ( too fragile or too stable)?  
 What expression levels characterizes a successful vs unsuccessful test?  
 Impact on section thickness?  
 Pattern on different assays?


In NordiQC run B34 10% of the participants used cell lines as onslide control

# Correlation of IHC for HER2 – accurate PATHWAY – cell lines and tissues

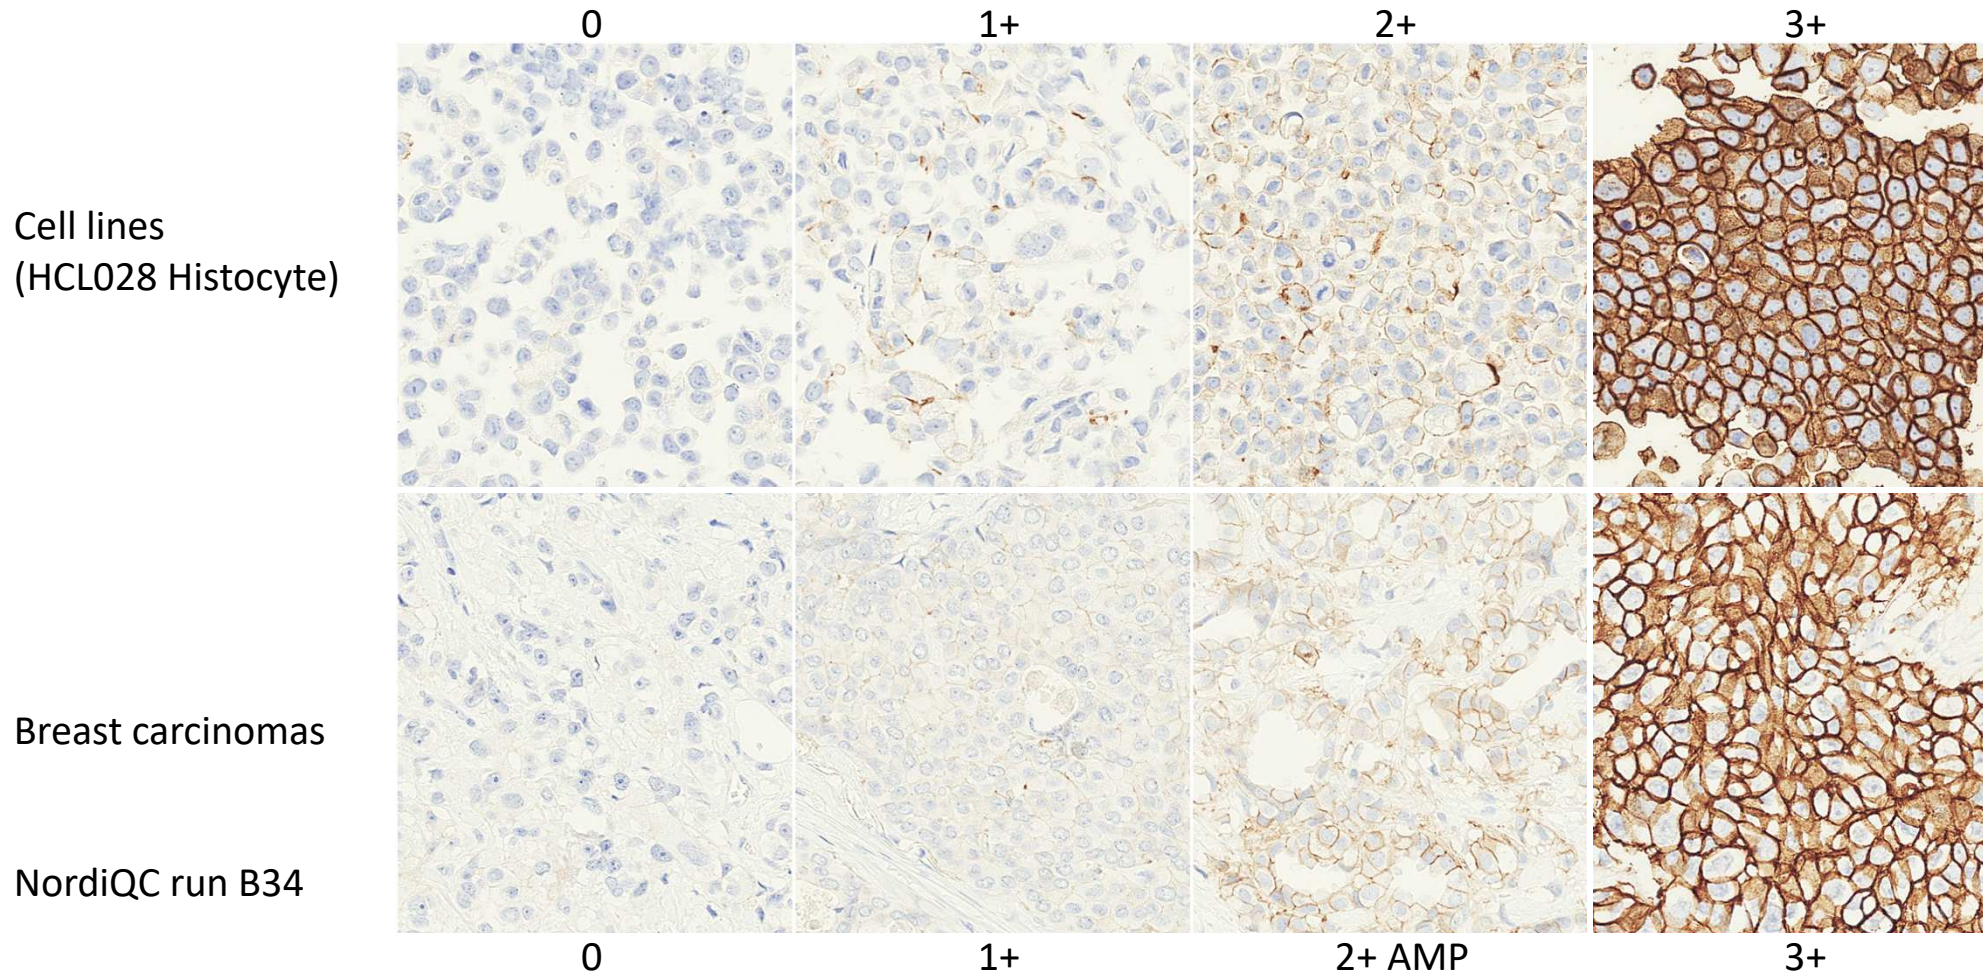





# Correlation of IHC for HER2 – (inaccurate) PATHWAY – cell lines and tissues

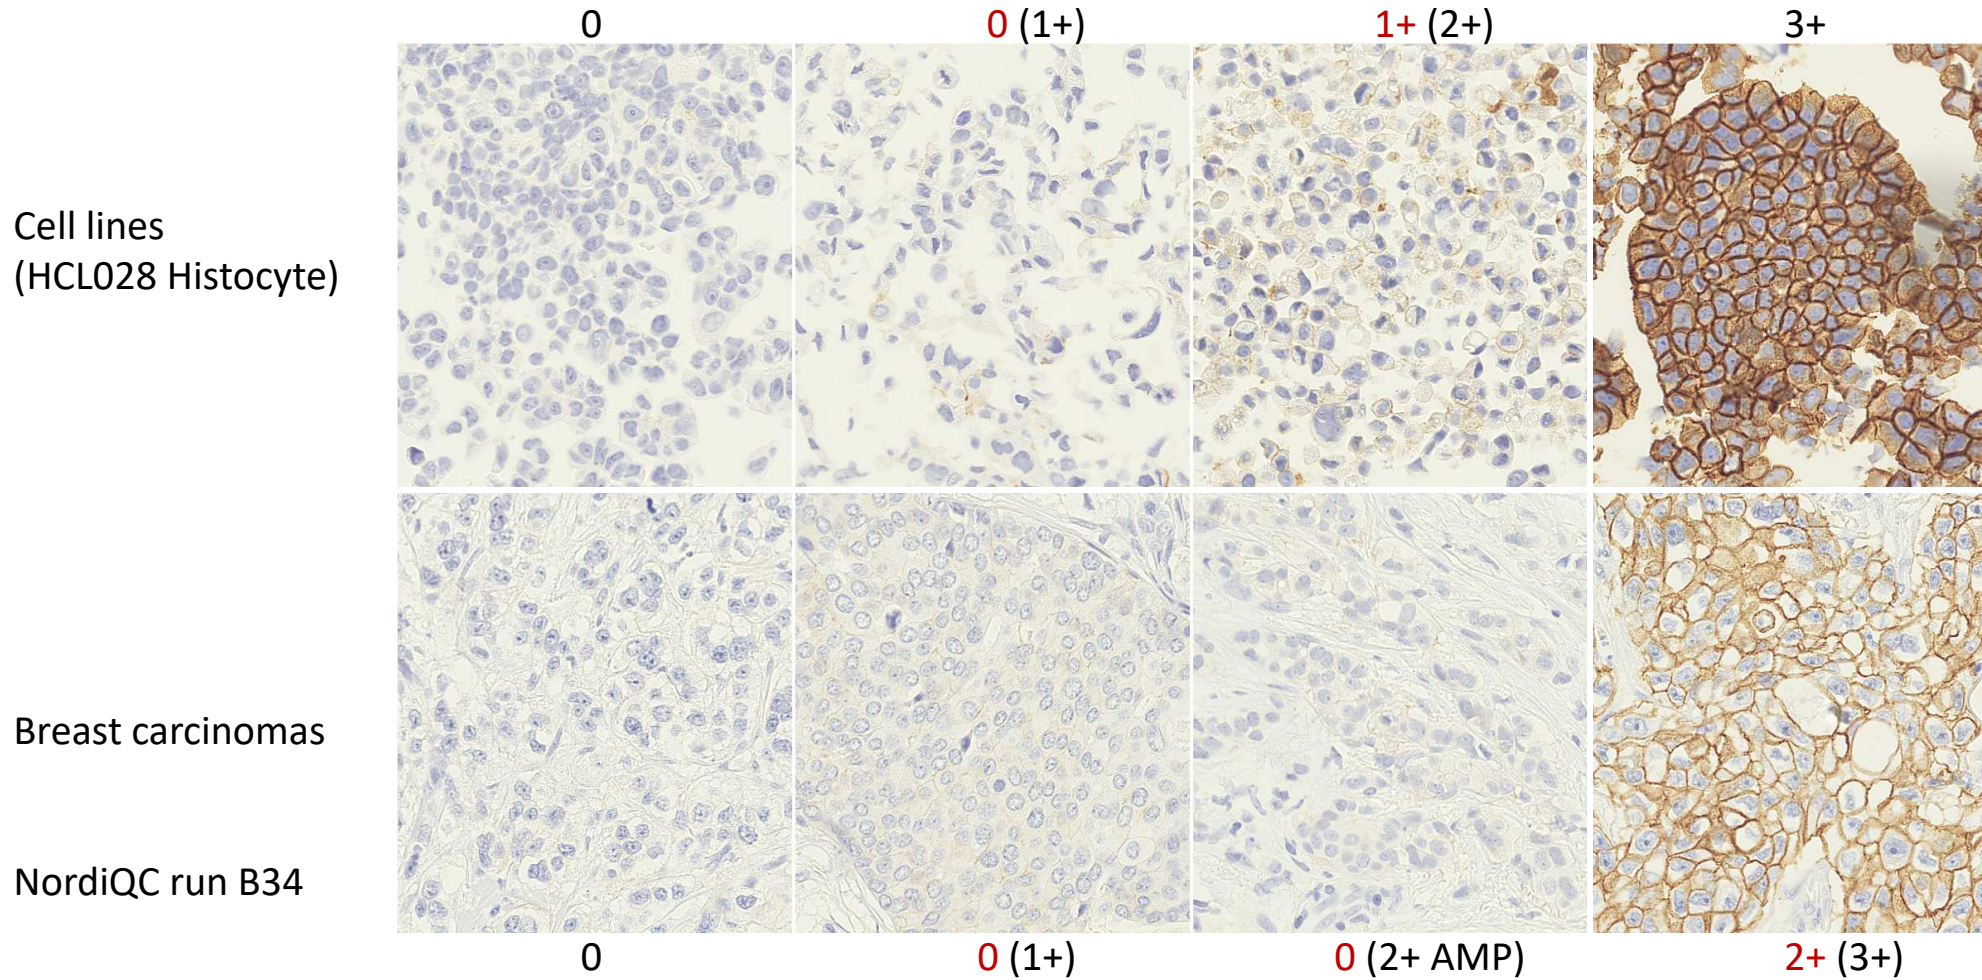

# Correlation of IHC for HER2 – HercepTest 2' Gen – cell lines and tissues

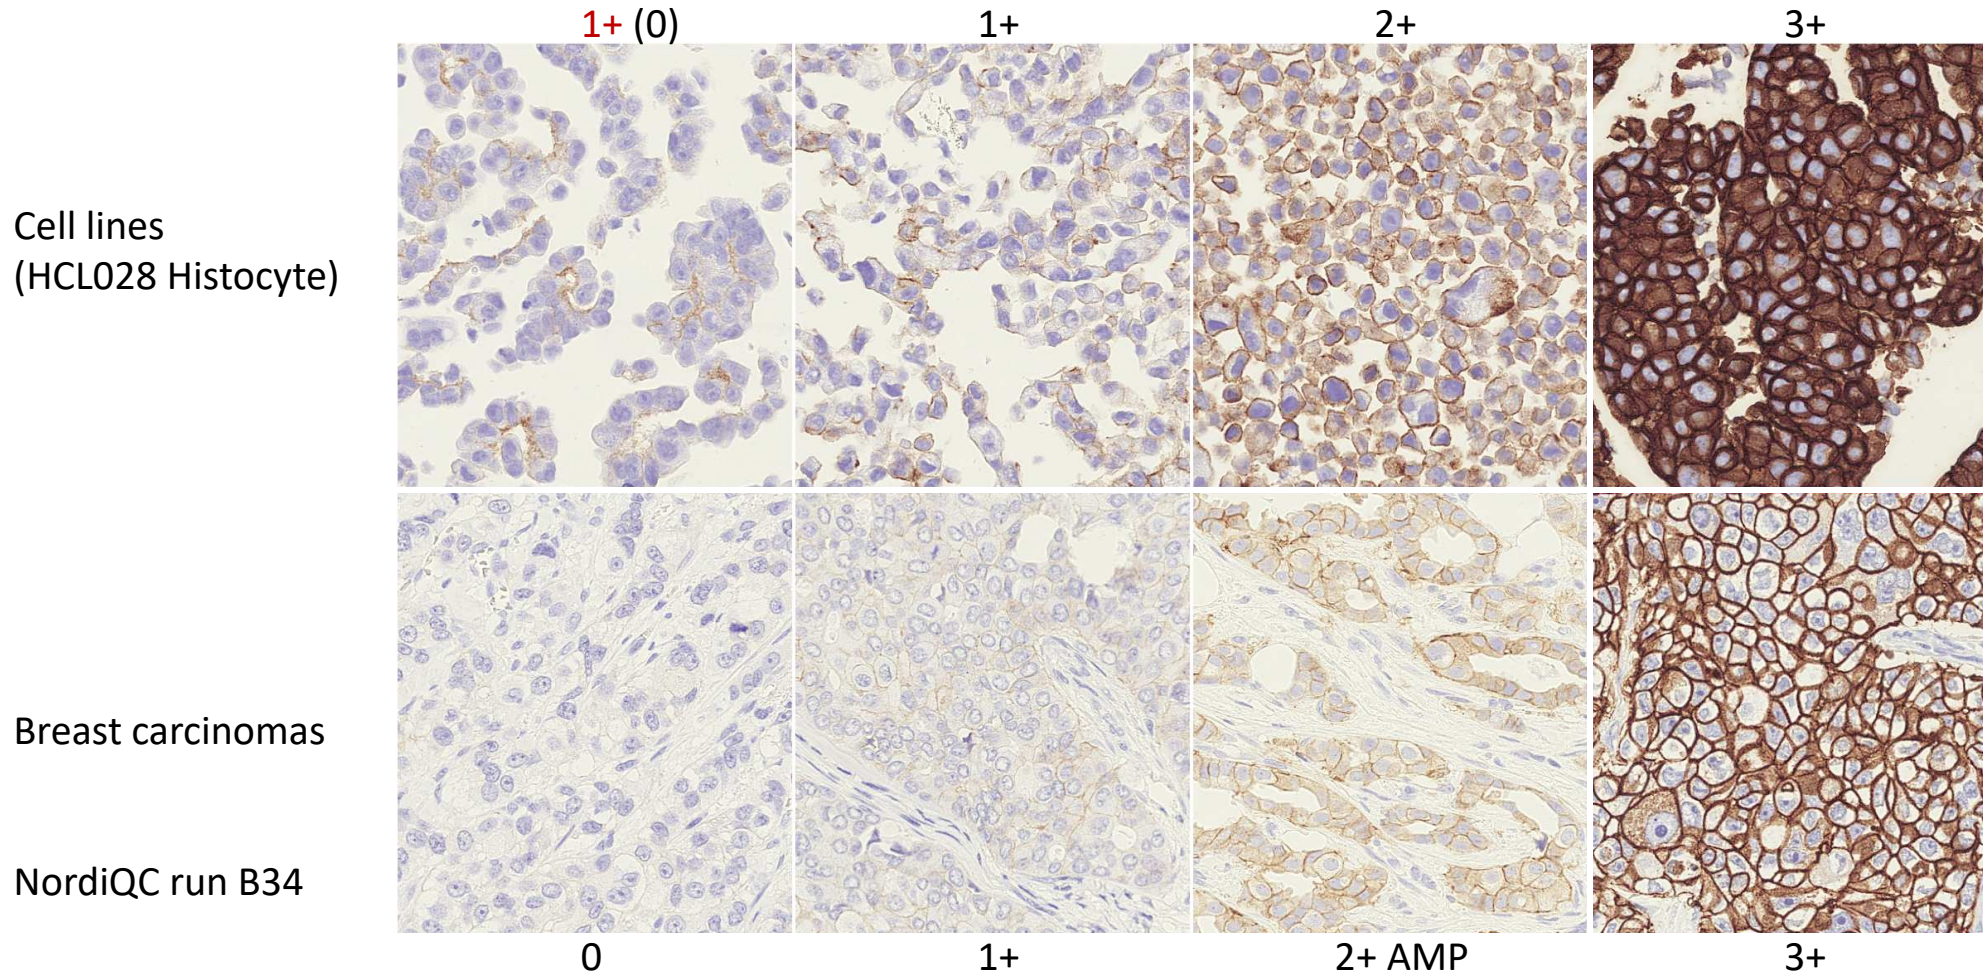

# Correlation of IHC for HER2 – SP3 – cell lines and tissues

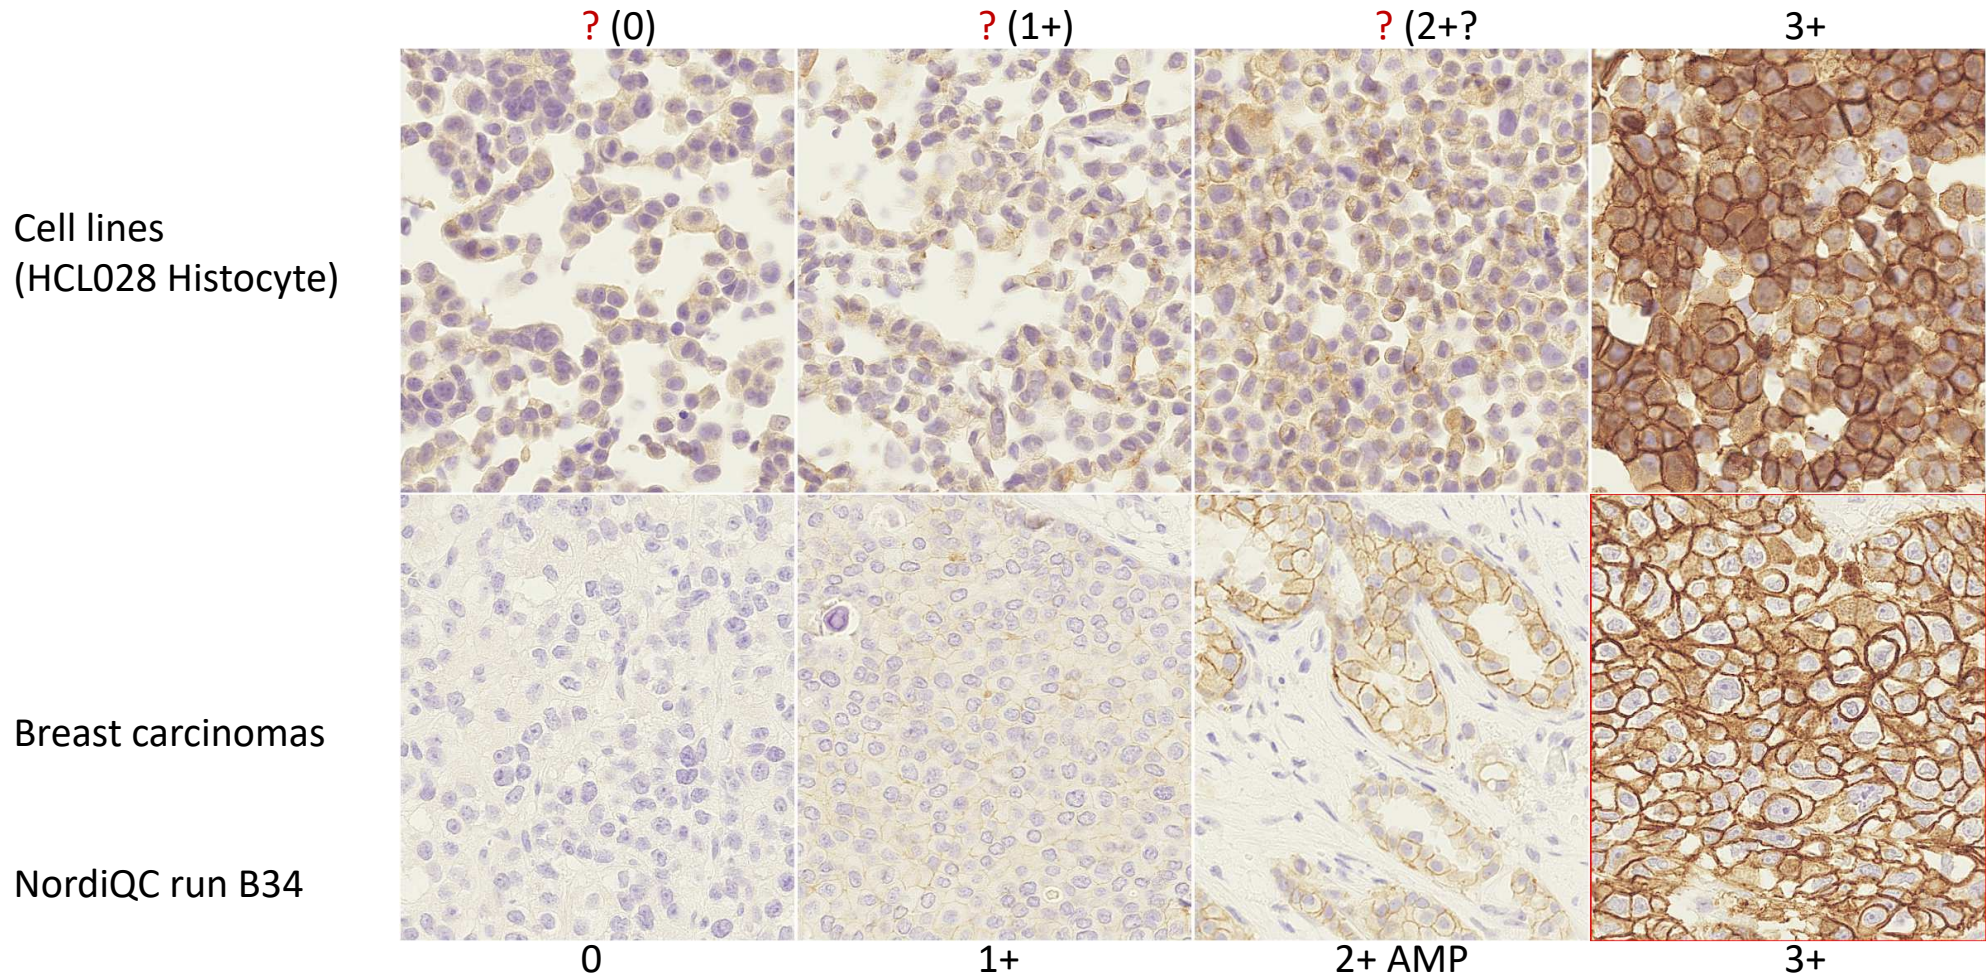


# Correlation of IHC for HER2 – cell lines and scoring

2+ weak


2+

2+

Cell lines  
(HCL028 Histocyte)

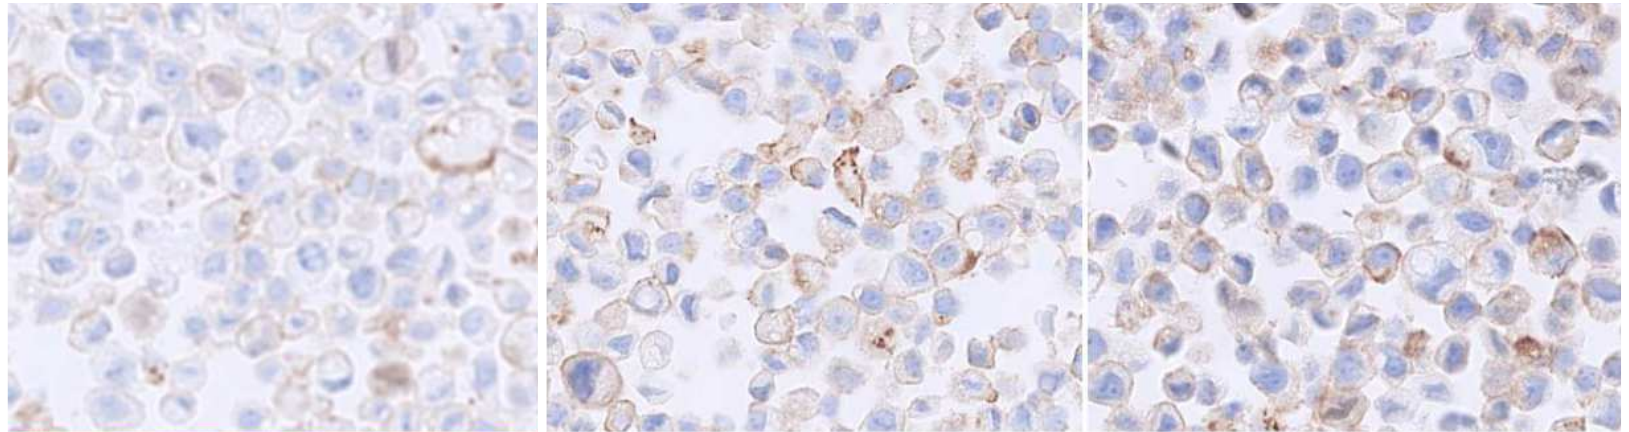

Breast carcinoma 1+

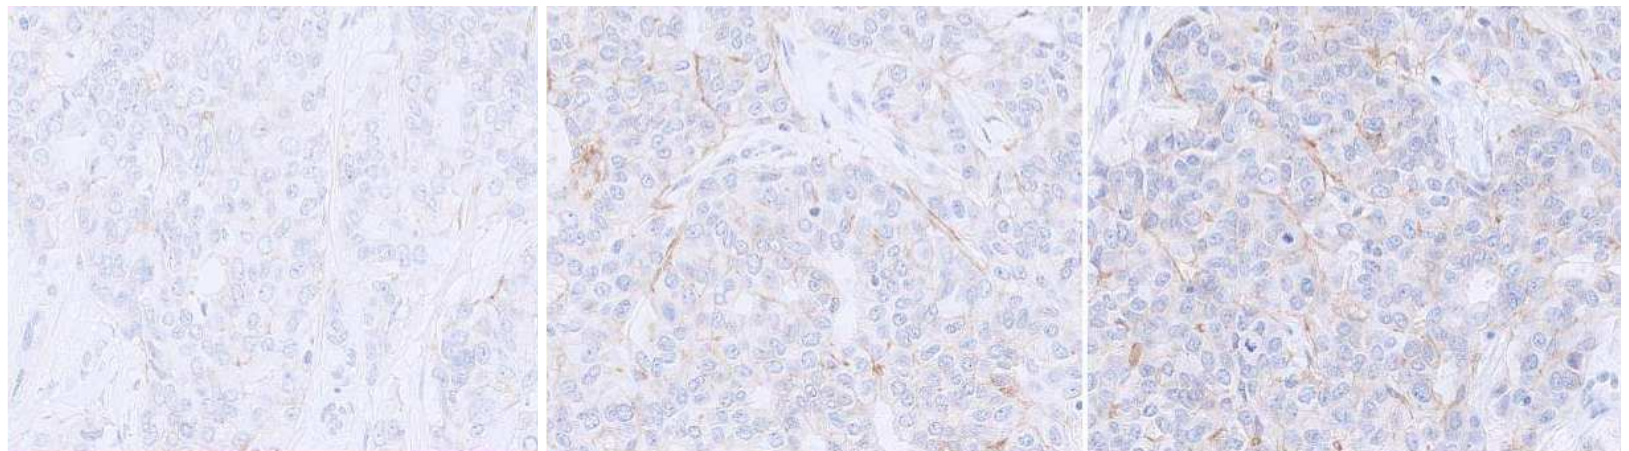


0

1+


1+

# The needs for cell lines as Quality tool for Accuracy/Precision


- Need to map staining characteristics for most commonly used IHC assays
  - The different assays will provide different patterns

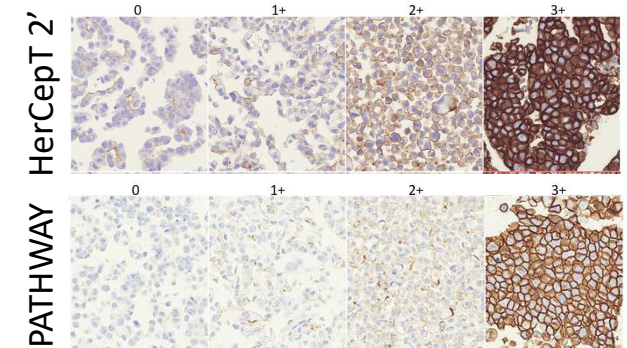

- Need to identify change in patterns being critical with risk of false negative / false positive results
  - Each assay most likely will have different patterns / thresholds

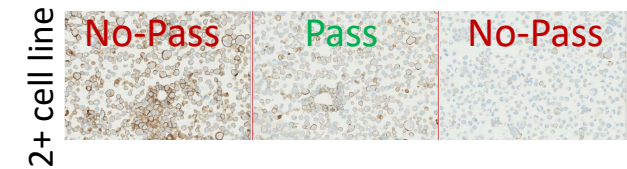

- Need to integrate software as digital image analysis (DIA) or artificial intelligence (AI) to secure reproducibility
  - Identification of DIA/AI QC-score for successful versus unsuccessful test

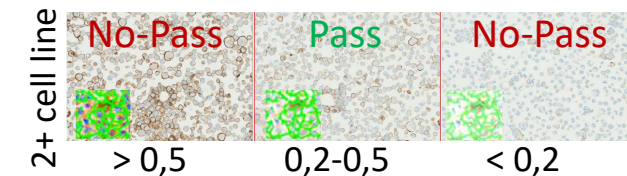


- The DIA/AI QC-scores must be validated for each IHC assay both with focus on expected level and critical levels
  - Large scale testing on e.g. breast carcinomas with the dynamic and critical range of the target analyte
  - Both to identify e.g. "classical" HER2 overexpression and the novel HER2 low category

# Analytical standards – IHC versus clinical chemistry; Calibrators

CA125; 35u/ml

CA-19; 37-40u/ml

....

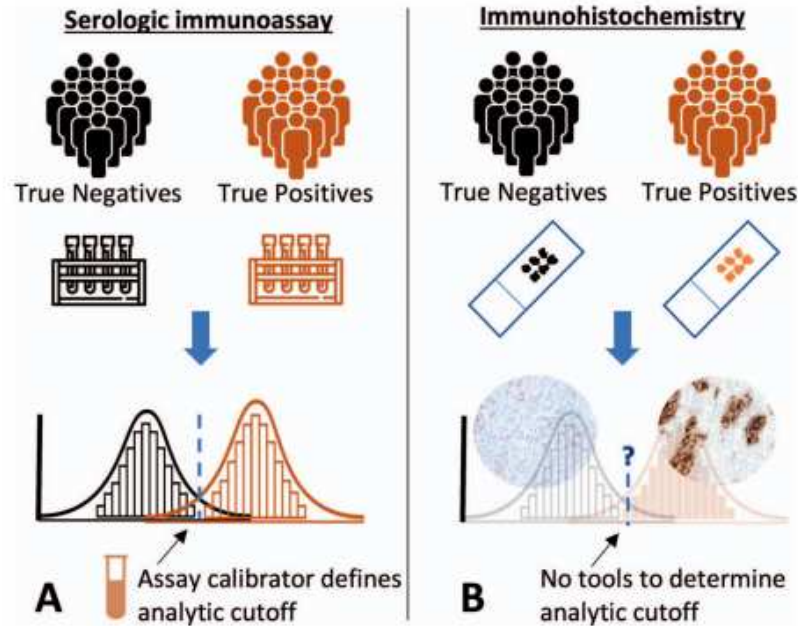


ICAPCs

But challenge for more semiquantitative biomarkers as especially HER2 and PD-L1...

## A Consortium for Analytic Standardization in Immunohistochemistry

Steven A. Bogen, MD, PhD; David J. Dabbs, MD; Keith D. Miller, FIBMS; Søren Nielsen, BLS; Suzanne C. Parry, BSc(Hons), MSc, FIBMS; Matthias J. Szabolcs, MD, PhD; Nils t'Hart, MD, PhD; Clive R. Taylor, MD, PhD; Emina E. Torlakovic, MD, PhD



(Arch Pathol Lab Med. doi: 10.5858/arpa.2022-0031-RA)

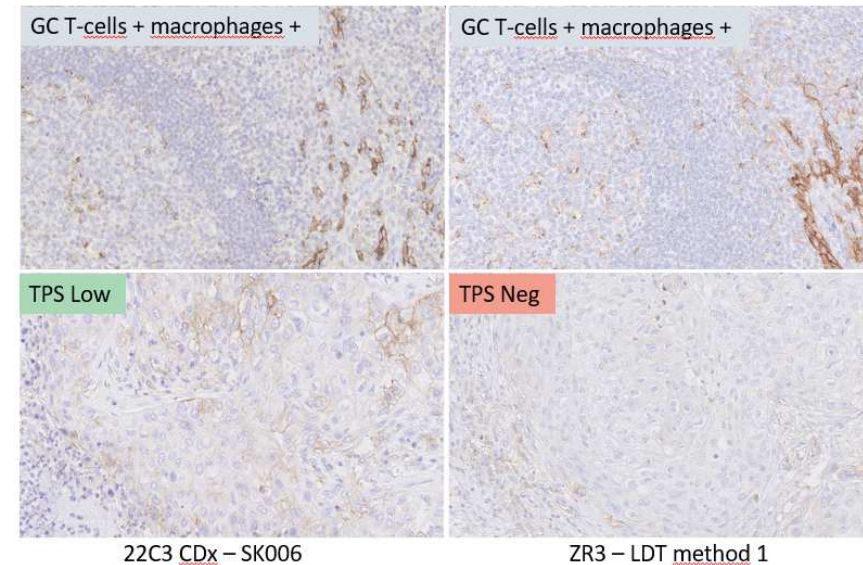



# Analytical standards – IHC versus clinical chemistry; Calibrators

Developmental and validation phase to correlate LOD\*/analytical sensitivity in microbeads versus diagnostic accuracy and sensitivity for;

ER, HER2, PD-L1 and p53

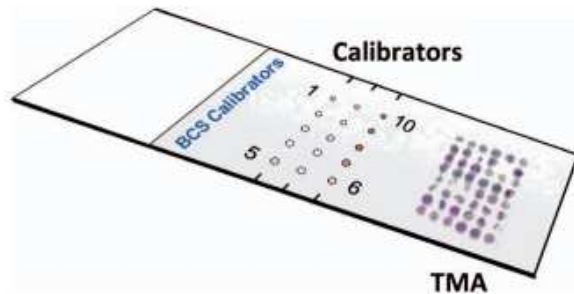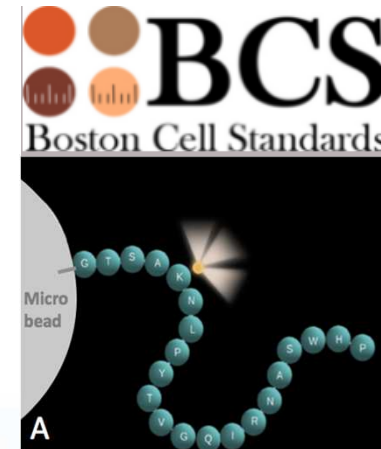

**Figure 5.** Illustration of the survey tool for correlating clinical accuracy (from the tissue microarray data) with analytic sensitivity (from the calibrator data). The calibrators are at up to 10 different concentrations; for example levels 1–10. The middle row depicts negative controls. Abbreviations: BCS, Boston Cell Standards; TMA, tissue microarray.

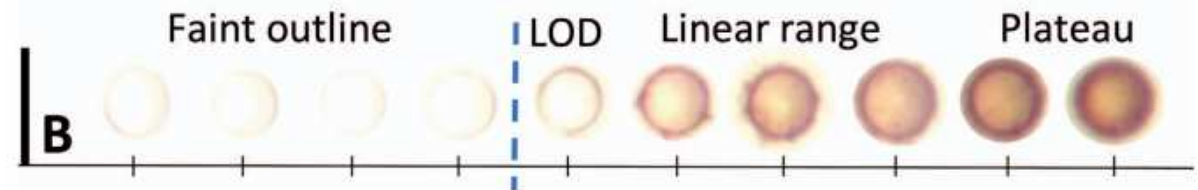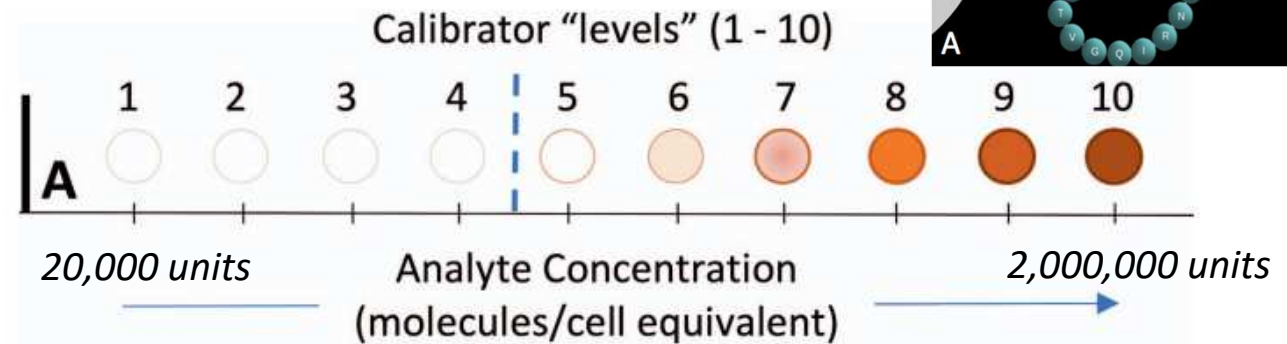

**Figure 2.** Illustration of a series of immunohistochemistry calibrators after staining. The numbers refer to calibrator levels, from low (1) to high (10) analyte concentrations. A, The illustration shows that rim staining is stronger than central staining because the analyte is attached to the microbead surface. In this example, level 5 represents the lower limit of detection (LOD). B, Images of microbeads from calibrators with an LOD at level 5.

## A Consortium for Analytic Standardization in Immunohistochemistry

Steven A. Bogen, MD, PhD; David J. Dabbs, MD; Keith D. Miller, FIBMS; Søren Nielsen, BLS; Suzanne C. Parry, BSc(Hons), MSc, FIBMS; Matthias J. Szabolcs, MD, PhD; Nils t'Hart, MD, PhD; Clive R. Taylor, MD, PI; Emina E. Torlakovic, MD, PhD

(Arch Pathol Lab Med. doi: 10.5858/arpa.2022-0031-RA)

# Reference standard materials for IHC; Calibrators – LOD\* - PD-L1



## CERTIFICATE OF ANALYSIS



\* LOD; Limit of detection / level of analytical sensitivity

**DESCRIPTION**  
 Product Description: IHCalibrators (10 levels)  
 Mean Diameter: 7-8 micron  
 Target: PD-L1 (extracellular Domain)

**CONCENTRATION**

Average PD-L1 Molecules per Microbead	Value
Level 10	603,077
Level 9	598,591
Level 8	479,714
Level 7	356,351
Level 6	228,502
Level 5	116,354
Level 4	53,551
Level 3	22,149
Level 2	9,550*
Level 1	2,197*

\*The values of levels 1 and 2 are estimates based on the amount of PD-L1 and from higher levels. The concentrations were too low for direct measurement

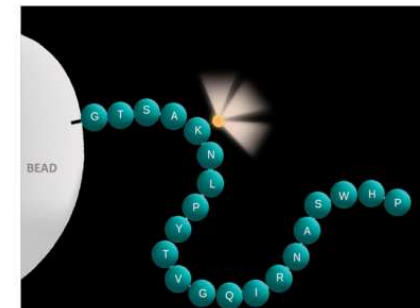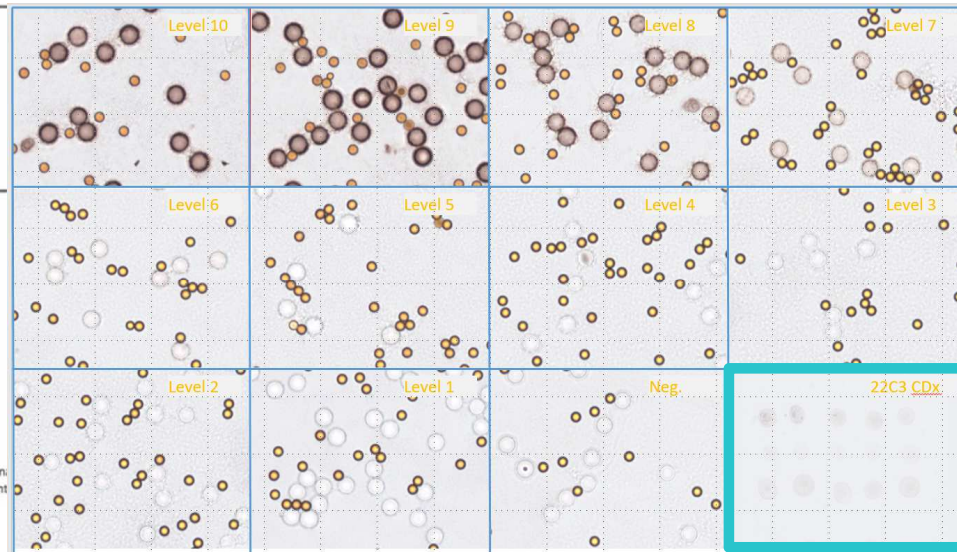

Bogen, SA. 2019. A root cause analysis into the high error rate in clinical immunohistochemistry. *Appl. Immunohistochem. Mol. Morphol.* 27(5) 329-338.

Sompuram, SR, K Vani, AK Schaedle, A Balasubramanian, & SA Bogen. 2019. Selecting an optimal positive IHC control for verifying retrieval. *J. Histochem. Cytochem.* 67(4):273-283.

Sompuram, SR, K Vani, AK Schaedle, A Balasubramanian, & SA Bogen. 2018. Quantitative assessment of immunohistochemistry laboratory performance by measuring analytic response curves and limits of detection. *Arch Pathol Lab Med.* 142 (7):851-862.



# Reference standard materials for IHC; Calibrators – LOD – PD-L1 22C3


ARTICLE OPEN

Check for updates

## Quantitative comparison of PD-L1 IHC assays against NIST standard reference material 1934

Seshi R. Sompuram<sup>1</sup>, Emina E. Torlakovic<sup>2,3</sup>, Nils A. 't Hart<sup>4</sup>, Kodela Vani<sup>1</sup> and Steven A. Bogen<sup>1</sup>


© The Author(s), under exclusive licence to United States & Canadian Academy of Pathology 2021, corrected publication 2021

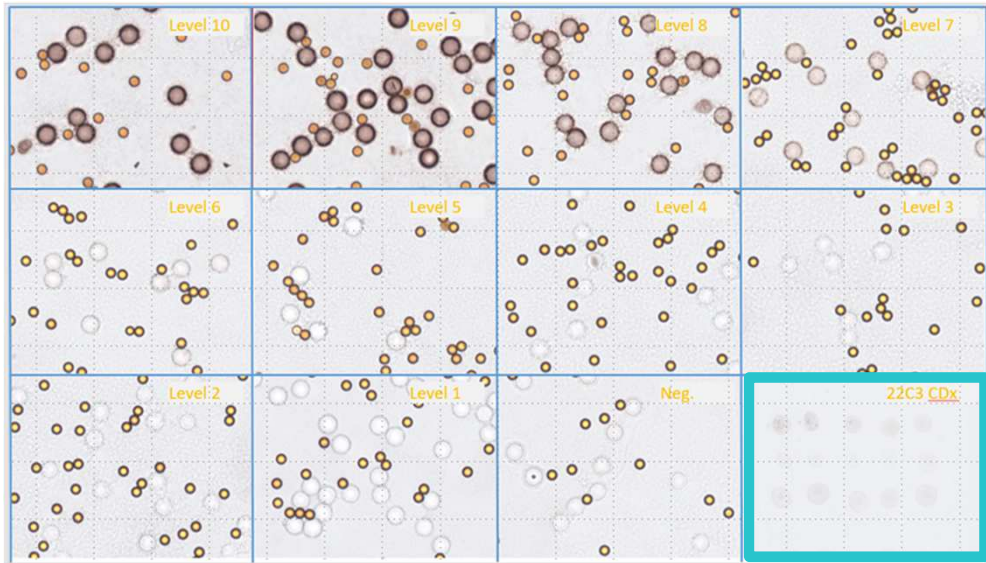

22C3 LOD  
356.351 mol.  
pr microbead

Average PD-L1 Molecules per Microbead


Level 10	603,077
Level 9	598,591
Level 8	479,714
Level 7	356,351
Level 6	228,502
Level 5	116,354
Level 4	53,551
Level 3	22,149
Level 2	9,550*
Level 1	2,197*

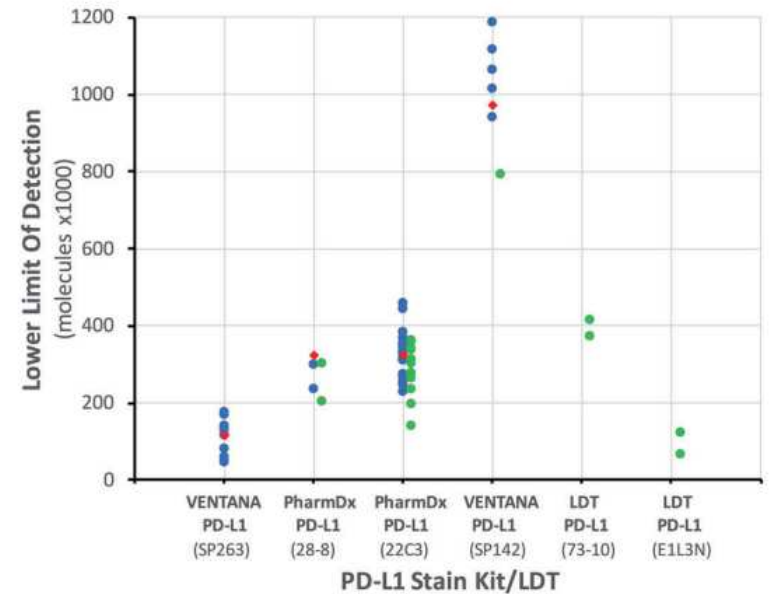

**Fig. 2 Lower limit of detection (LOD) of various PD-L1 assays (x axis).** Lower numbers (on the y axis) equate to greater sensitivity. Each dot represents a separate IHC laboratory test. Blue dots depict FDA-cleared assays in clinical laboratories, green dots for laboratory-developed tests (LDTs), and red diamonds for FDA-cleared assays as performed by a reference laboratory. Tissue staining in Fig. 2 was performed by these reference labs. For enhanced clarity, the LDT data are positioned slightly to the right of the vertical lines.

*Mod Pathol.* 2022;35(3):326–332.


# IHC Calibrator 10 levels HER2 – Boston Cell Standards - PATHWAY

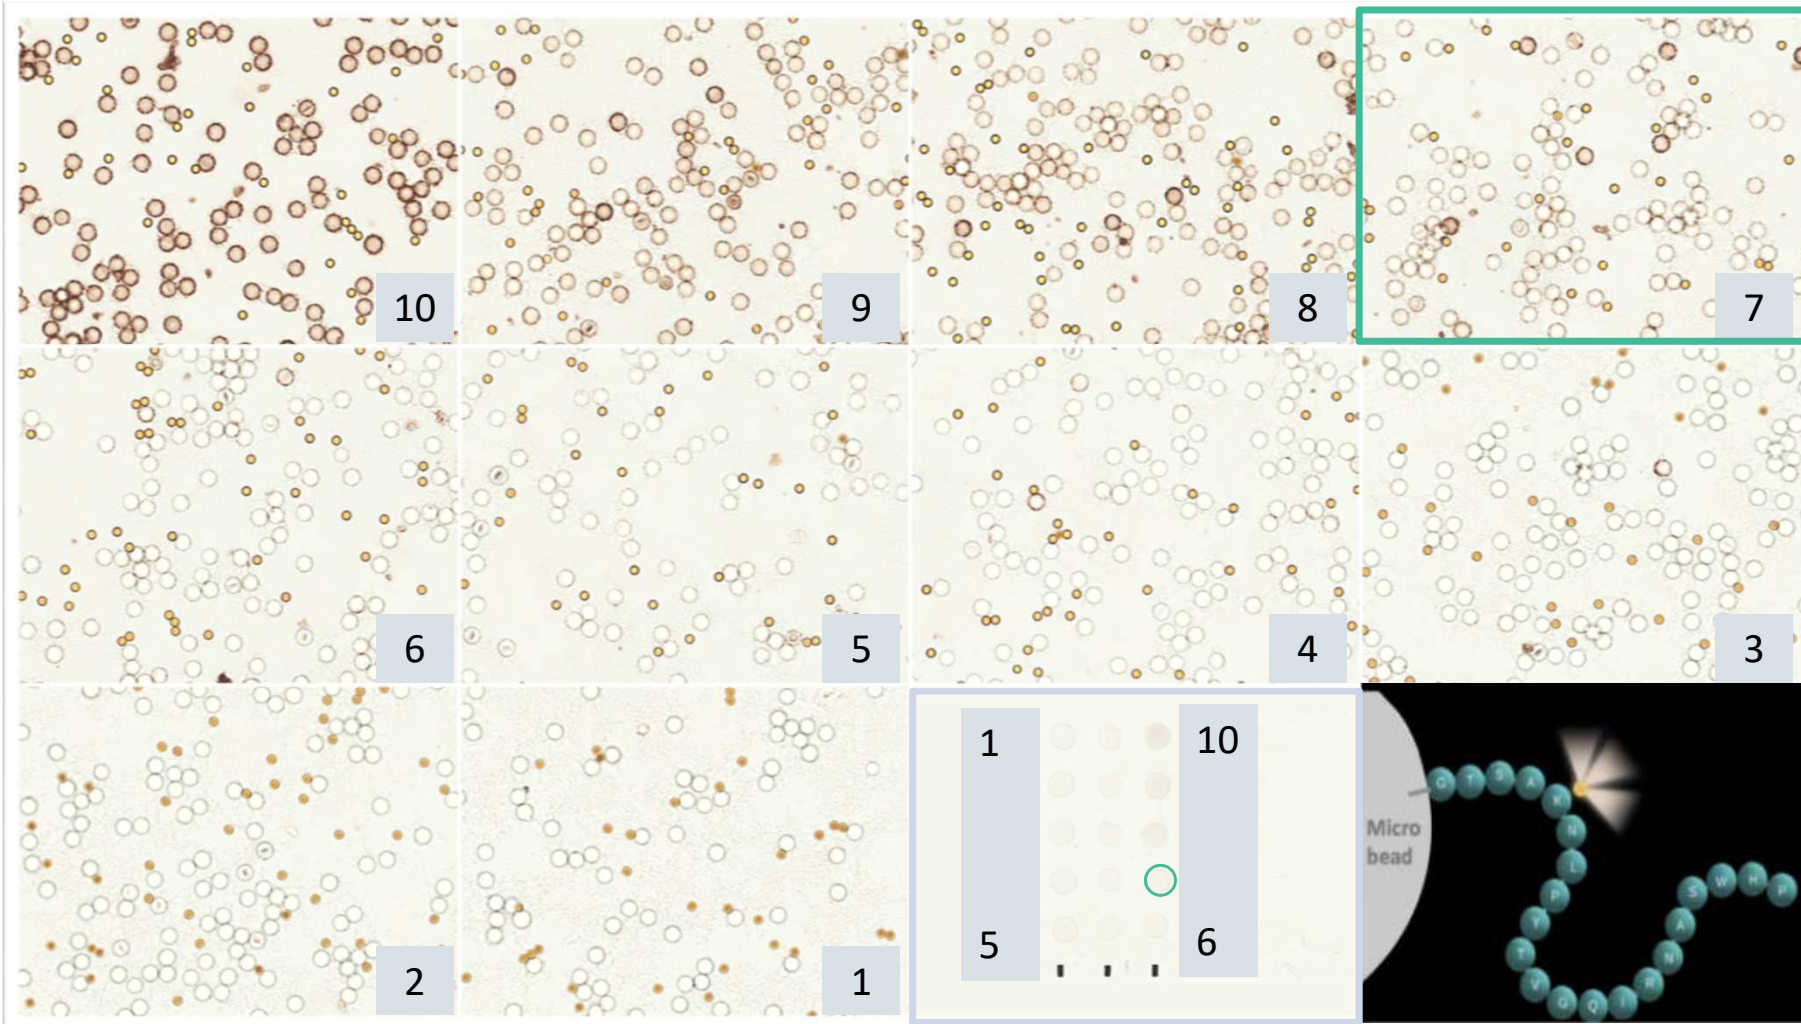

HER2 molecules  
pr microbead

- 10. >2,715,976
- 9. 2,715,976
- 8. 2,669,835
- 7. 1,981,264**
- 6. 1,274,947
- 5. 724,800
- 4. 376,965
- 3. 206,597
- 2. 114,315
- 1. 62,849

# Correlation of IHC for HER2 – Microbeads – Accuracy/Precision



HER2 molecules  
pr microbead

8. 2,669,835










7. 1,981,264

6. 1,274,947


PATHWAY Standard

PATHWAY – red. HIER & Ab

PATHWAY + OptiView

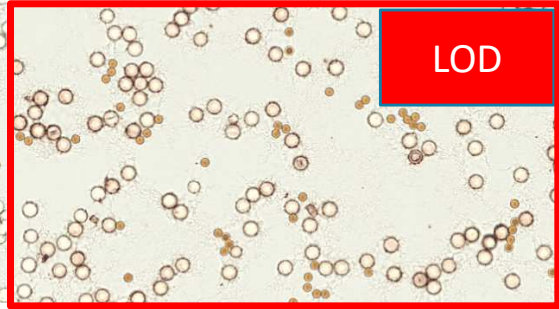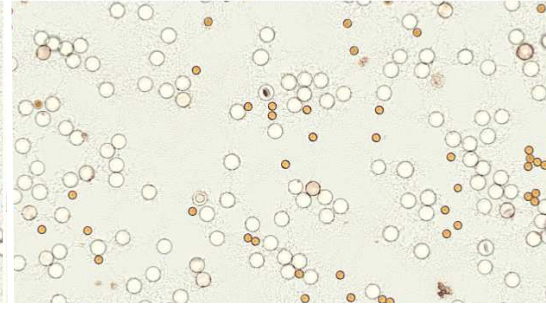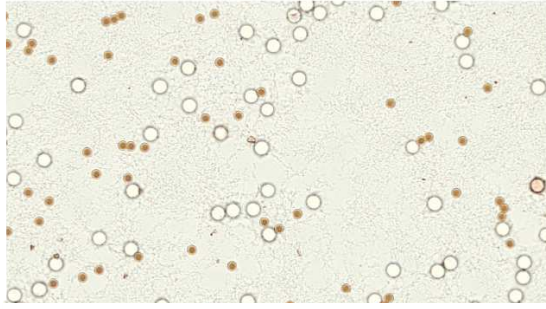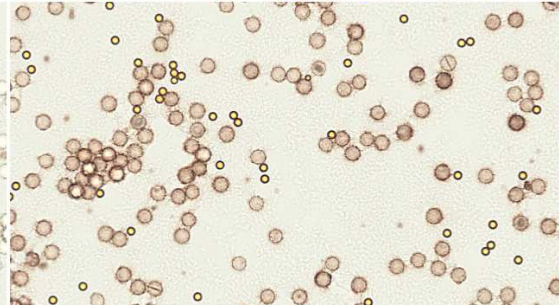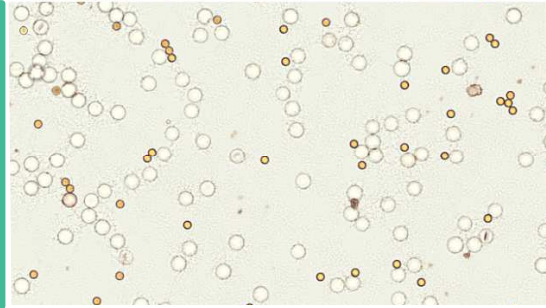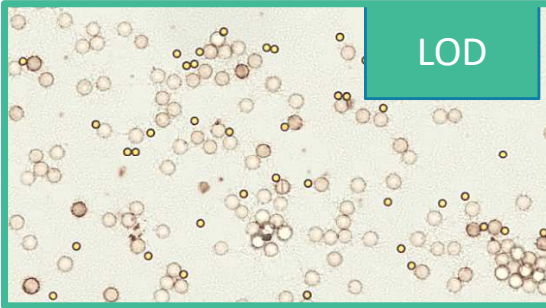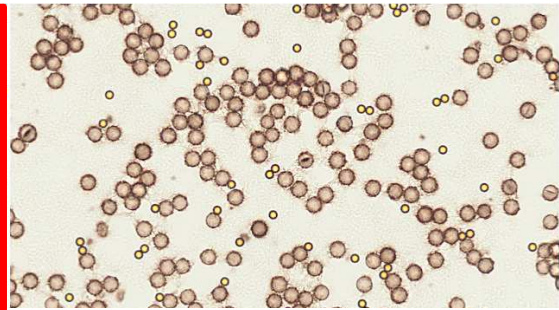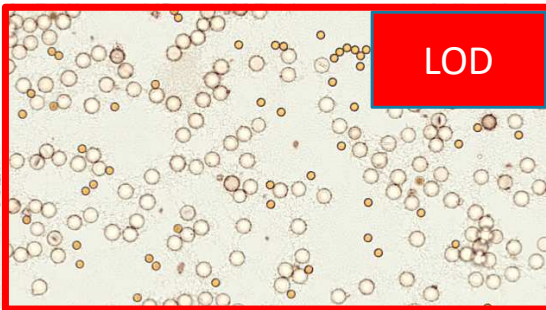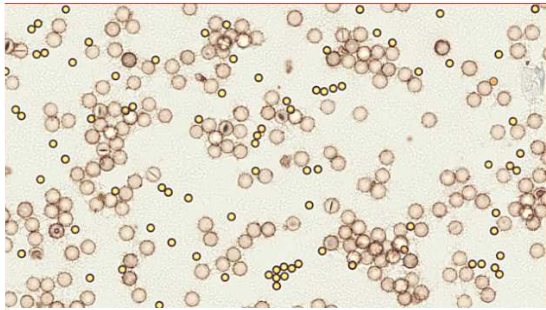

# Correlation of IHC for HER2 – Microbeads – Accuracy/Precision






Breast carcinomas

PATHWAY Standard  
LOD 1.981.264 HER2 mol.




PATHWAY – red. HIER & Ab  
LOD 2.669.835 HER2 mol.

PATHWAY + OptiView  
LOD 1,274,947 HER2 mol.




Unamplified 1+

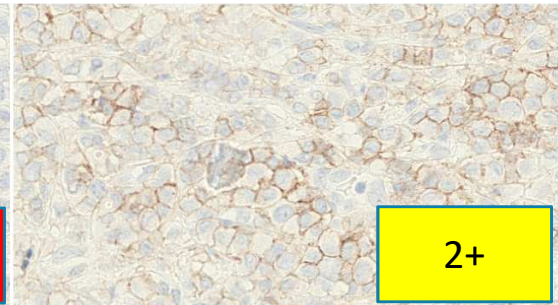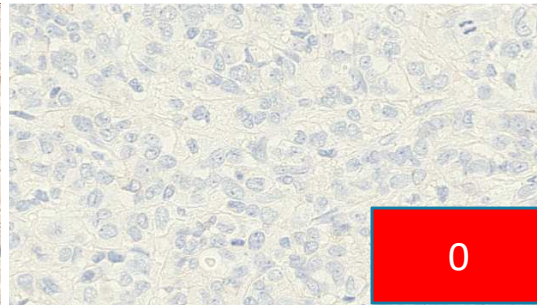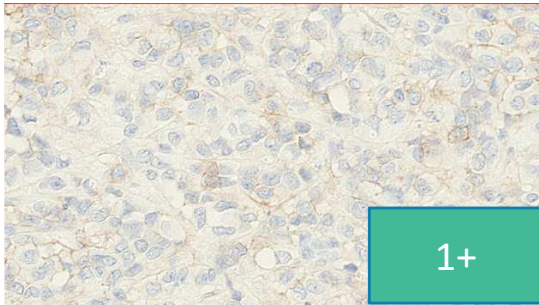


Amplified 2+

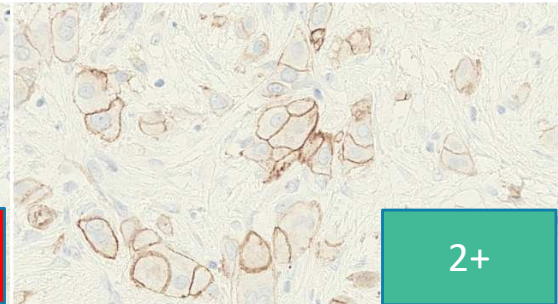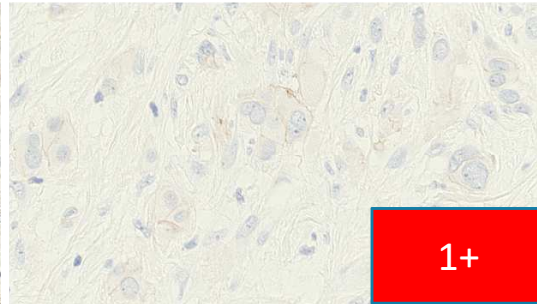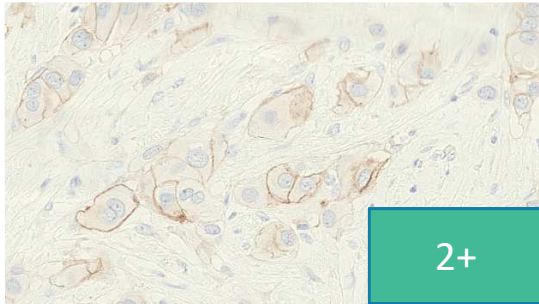

Amplified 3+

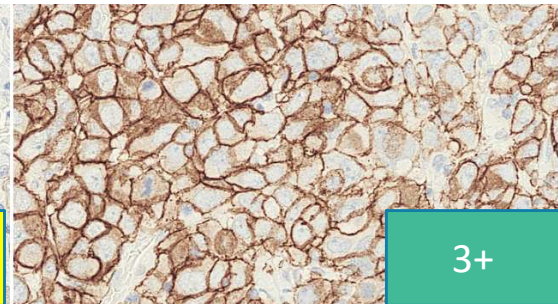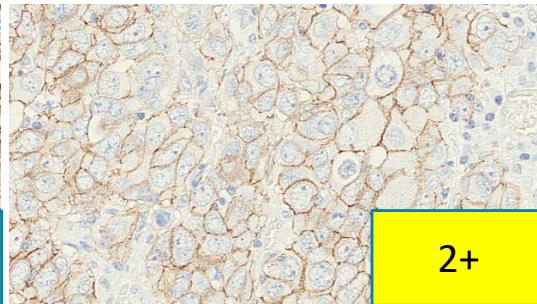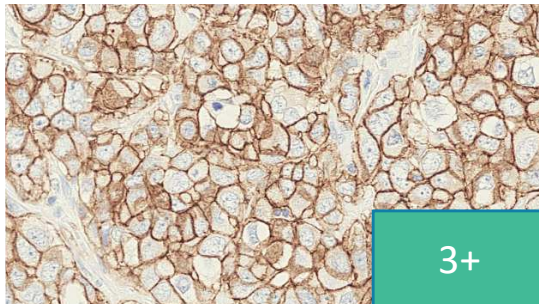

# Correlation of IHC for HER2 – Microbeads – Accuracy/Precision



Breast carcinomas


N=15 (NordiQC runs B31, B32, B33)

			PATHWAY Standard LOD 1,981,264 HER2 mol.	PATHWAY – red. HIER & Ab LOD 2,669,835 HER2 mol.	PATHWAY + OptiView LOD 1,274,947 HER2 mol.
HER2 classical	HER2 Low	0	2	5	0
		1+	3	3	3
		2+ Unamplified	1	2	3
		2+ Amplified	3	1	3
		3+ Amplified	6	4	6

Reduced analytical sensitivity (LOD) provided a less accurate HER2 result for both classical overexpression and HER2 low

Increased analytical sensitivity (LOD) provided a less accurate HER2 result for HER2 low

# IHC Calibrator 10 levels HER2 – Boston Cell Standards – HercepTest Mo.

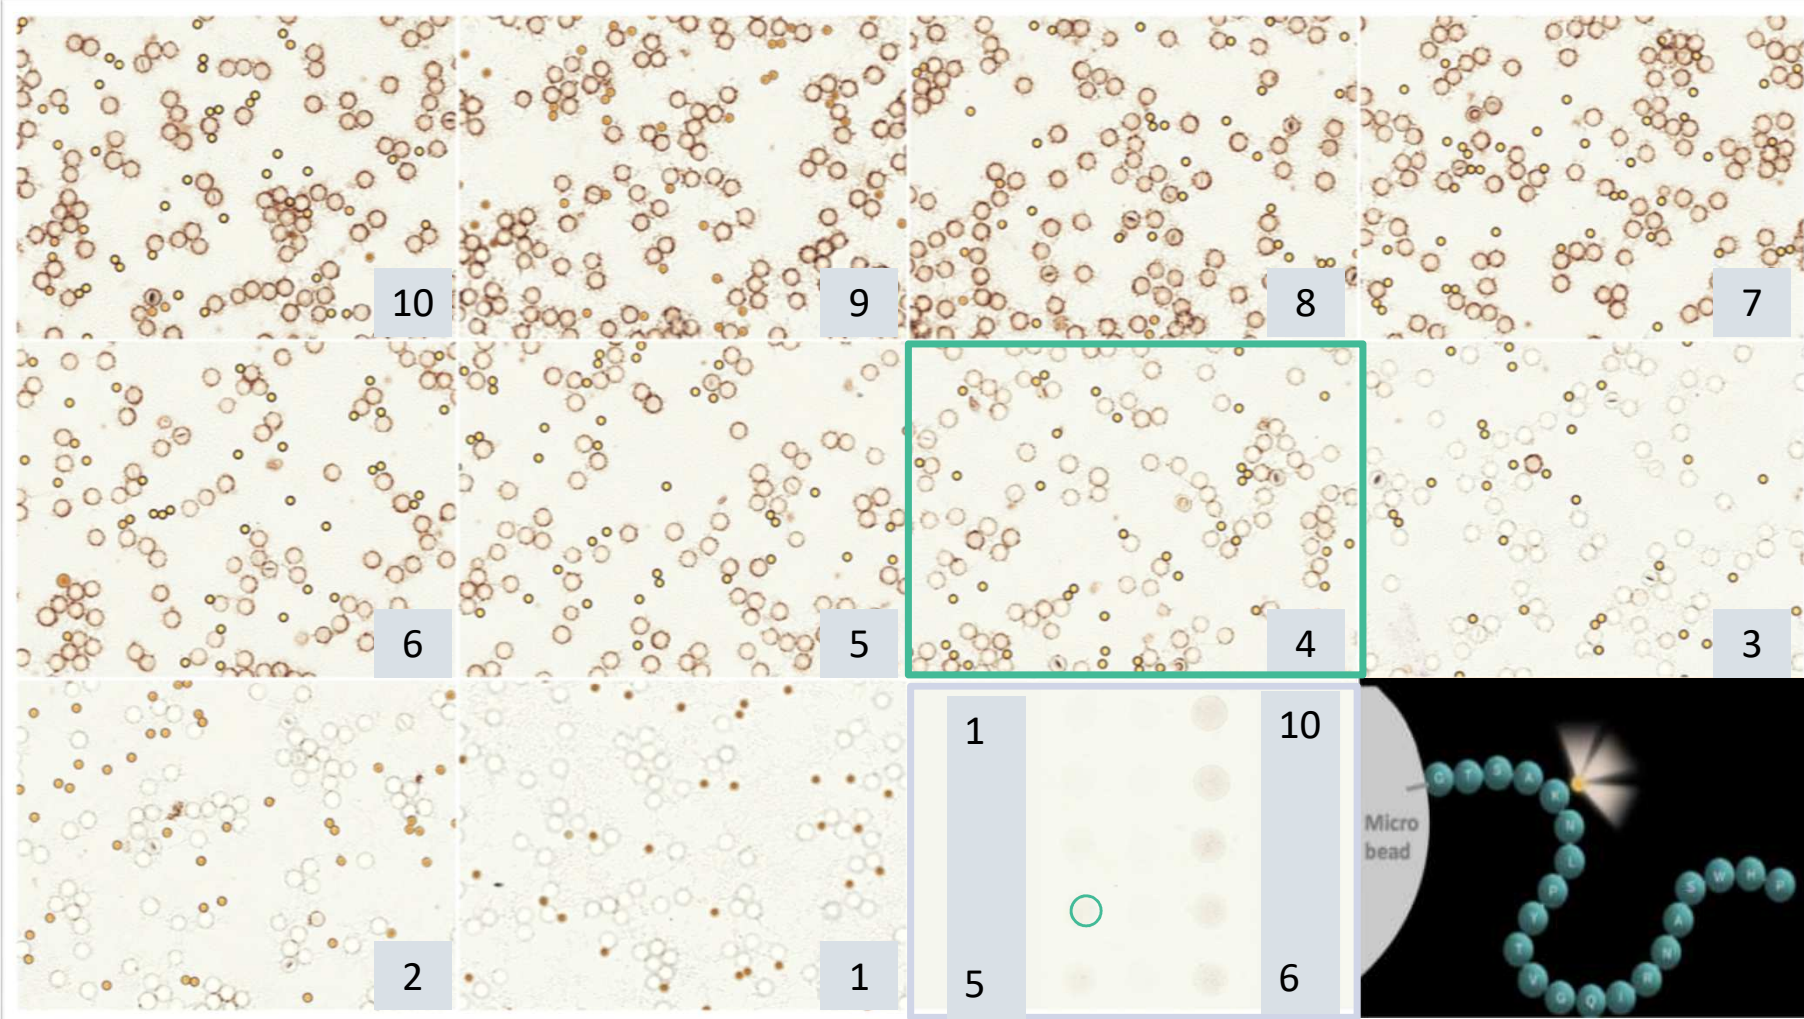

HER2 molecules  
pr microbead

- 10. >2,715,976
- 9. 2,715,976
- 8. 2,669,835
- 7. 1,981,264
- 6. 1,274,947
- 5. 724,800
- 4. 376,965**
- 3. 206,597
- 2. 114,315
- 1. 62,849

## Standardized controls for Immunohistochemistry

- Precision testing for precision medicine needs precision IHC controls
- At present no "golden standard IHC controls" to fit all IHC biomarkers
- A mixture of carefully selected external tissue controls and non-tissue based controls as cell lines and/or microbeads seem to be best practice
- Cell lines and microbeads have potential to monitor IHC test precision and accuracy, BUT still require extensive documentation and data how to use these

*Different performances related to IHC assays*


*Different thresholds for adequate vs inadequate result*

*Software DIA/AI QC-tools to be developed and verified*

# Application of TMA for QC of diagnostic IHC

Daily IHC control for the majority of routine markers:

Appendix  
Liver  
Pancreas  
Tonsil

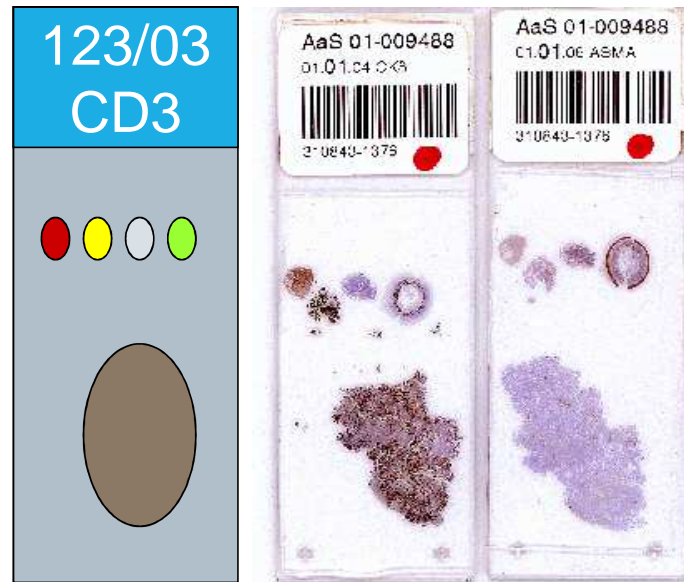

Each slide stained and evaluated has essential information of the obtained sensitivity and specificity

In contrast only using 1 external tissue run control, no information is available for the single slide evaluated



# Application of TMA for QC of diagnostic IHC

	TMA On-slide control	TMA Run / batch control	Remarks
Missing reagent FN in patient test	Yes	No – only control slide	Potential internal pos. control only indicator of protocol performed
Wrong antibody FP in patient test	Yes	No – only control slide	
Inappropriate protocol performance - Drying out etc FN / FP in patient test	Yes	No – only control slide	Potential internal pos. control only indicator of protocol performed
	Errors seen for all IHC automated and semi-automated IHC platforms		

# On-slide controls....

## REVIEW ARTICLE

(*Appl Immunohistochem Mol Morphol* 2015;23:1–18)

### Standardization of Positive Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Committee

Emina E. Torlakovic, MD, PhD,\*† Soren Nielsen, HT, CT,‡§ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),||\*# John Garratt, RT,†\*\* Blake Gilks, MD, FRCPC,††† Jeffrey D. Goldsmith, MD,‡‡ Jason L. Hornick, MD, PhD,\*§§ Elizabeth Hyjek, MD, PhD,\* Merdol Ibrahim, PhD,|| Keith Miller, FIBMS,|| Eugen Petcu, MD, PhD,|| Paul E. Swanson, MD,¶### Xiaoge Zhou, MD,\*\*††† Clive R. Taylor, MD, PhD,‡‡‡ and Mogens Vyberg, MD‡§

## RESEARCH ARTICLE

(*Appl Immunohistochem Mol Morphol* 2017;25:308–312)

### An Audit of Failed Immunohistochemical Slides in a Clinical Laboratory: The Role of On-Slide Controls


Carol C. Cheung, MD, PhD, JD,\*† Clive R. Taylor, MD, DPhil,‡ and Emina E. Torlakovic, MD, PhD†

## Estrogen and Progesterone Receptor Testing in Breast Cancer: ASCO/CAP Guideline Update

Kimberly H. Allison, MD<sup>1</sup>; M. Elizabeth H. Hammond, MD<sup>2</sup>; Mitchell Dowsett, PhD<sup>3</sup>; Shannon E. McKernin<sup>4</sup>; Lisa A. Carey, MD<sup>5</sup>; Patrick L. Fitzgibbons, MD<sup>6</sup>; Daniel F. Hayes, MD<sup>7</sup>; Sunil R. Lakhani, MD<sup>8,9</sup>; Mariana Chavez-MacGregor, MSc<sup>10</sup>; Jane Perlmutter, PhD<sup>11</sup>; Charles M. Perou, PhD<sup>2</sup>; Meredith M. Regan, ScD<sup>12</sup>; David L. Rimm, MD, PhD<sup>13</sup>; W. Fraser Symmans, MD<sup>10</sup>; Emina E. Torlakovic, MD, PhD<sup>14,15</sup>; Leticia Varella, MD<sup>16</sup>; Giuseppe Viale, MD<sup>17,18</sup>; Tracey F. Weisberg, MD<sup>19</sup>; Lisa M. McShane, PhD<sup>20</sup>; and Antonio C. Wolff, MD<sup>21</sup>

J Clin Oncol 38:1346-1366. © 2020 by American Society of Clinical Oncology

“even for automated stainers, where it cannot be guaranteed that every slide in fact receives identical treatment”.

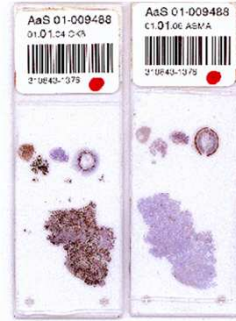

### Use of on-slide controls in NordiQC

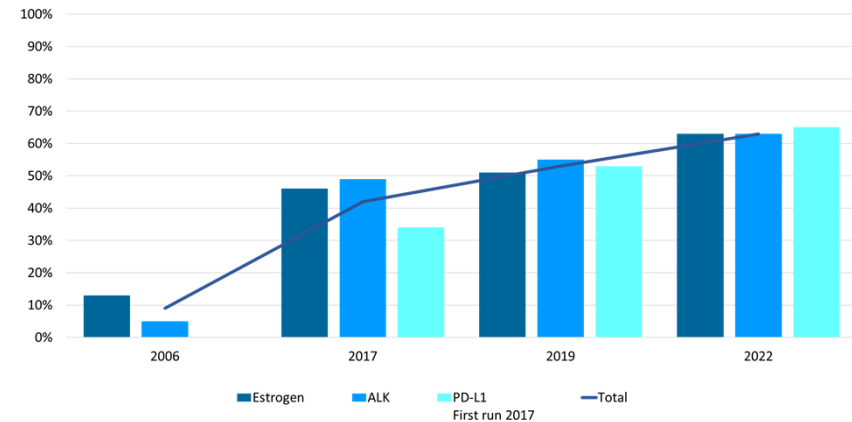


Fig. 5 Evolution of use of on-slide controls in NordiQC

Evolution in the Use of On-Slide Controls for Diagnostic Immunohistochemistry in the Era of Precision Testing  
Heidi Lykke Kristoffersen, Rasmus Røge, Søren Nielsen. NordiQC, Aalborg Universityhospital, Denmark.  
USCAP 2023


# Application of TMA for QC of diagnostic IHC

## RESEARCH ARTICLE

(*Appl Immunohistochem Mol Morphol* 2017;25:308–312)

### An Audit of Failed Immunohistochemical Slides in a Clinical Laboratory: The Role of On-Slide Controls

Carol C. Cheung, MD, PhD, JD,\*† Clive R. Taylor, MD, DPhil,‡ and Emina E. Torlakovic, MD, PhD†

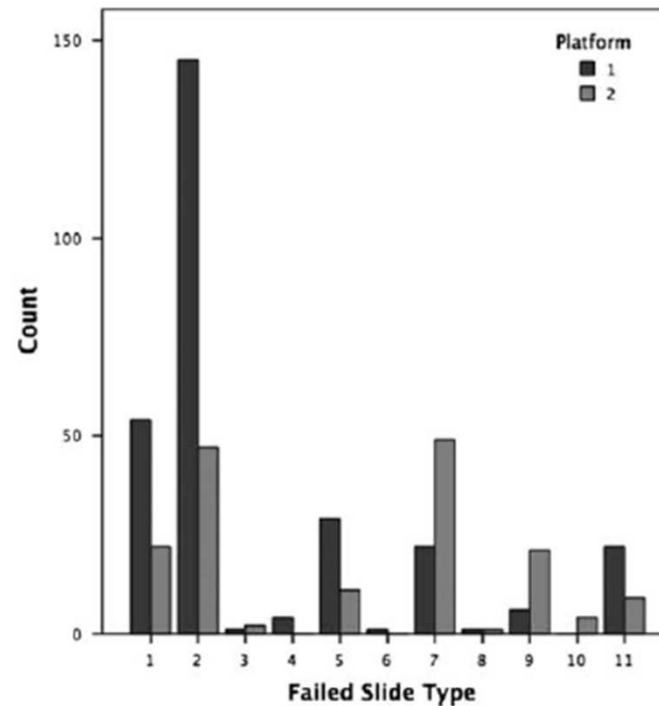

**FIGURE 1.** Frequency of failed immunohistochemistry slides by category and platform.

**TABLE 1.** Categories of Failed IHC Slides

Failed IHC Slide Category	Description	Comments
1	On-slide control too weak, patient tissue negative	Correct primary Ab was applied, but test sensitivity is possibly too low
2	On-slide control negative, patient tissue negative	Total slide failure; the result of the test does not suggest possible cause of the failure
3	On-slide control too weak, patient tissue weakly positive but no internal control	May indicate decreased technical sensitivity
4	On-slide control negative, patient tissue weakly positive but no internal control	There is uncertainty whether the correct primary Ab was applied or if there was significantly decreased sensitivity
5	No on-slide control, patient tissue negative	Uncertain results; cannot distinguish if the staining was optimal, suboptimal, or total failure
6	No on-slide control, patient tissue positive	No internal control present; lesion positive; failed only if there is uncertainty over whether the proper primary Ab was applied
7	Failed signal-to-noise ratio	Usually too high background; potential false positive, involving both patient sample and on-slide external control
8	Counter staining problem	If severe, may render result uninterpretable
9	Wrong protocol	Wrong protocol selected when > 1 protocol for the given primary Ab exists in the system
10	Uneven staining	Large or critical areas of the patient tissue or controls were missed by uneven staining
11	Wrong control	Either wrong tissue control or areas relevant to the test were missing (detached during staining or paraffin block with control tissue cut through)

IHC indicates immunohistochemistry.

2% error rate;

Class I 0,8%

Class II 9,0%

(452/22.234 slides)

# Application of TMA for QC of diagnostic IHC

## A: On-slide controls


IHC slides stained for ALK (Class II),  
same run, same instrument, same protocol  
14/19 passed  
5/19 failed (5 x 150 USD)

## B: Batch-control - Theoretically:

Batch control **failed** by same conditions as above  
0/19 passed  
19/19 failed (no consistent internal control...) (20 x 150 USD)

## C: Batch-control - Theoretically:

Batch control **passed** by same conditions as above  
19/19 passed  
0/19 failed (the 5 failed slides not identified....) (Cost...???)

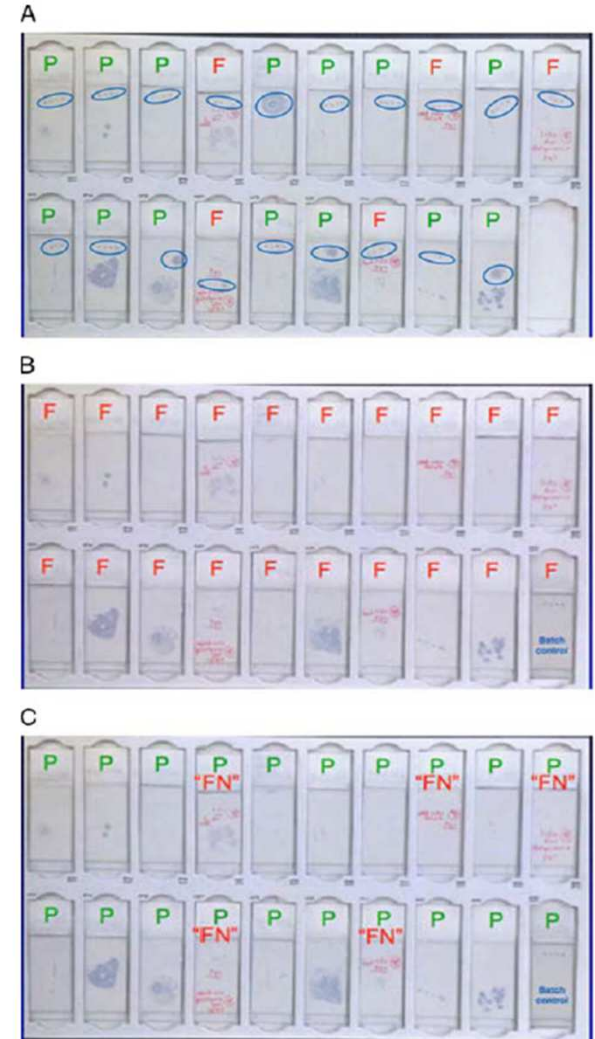

# Conclusions

Focus on external tissue controls is central to standardize and optimize IHC:

- On-slide TMA controls are preferable to 1 batch control
- Internal tissue controls are of limited value
- Need to generate consensus guidelines on ICAPCs for all IHC tests – which tissues, which staining pattern. Interaction of industry, EQA and pathology organisations and societies required.
- Need to identify best practice controls – tissues, beads, cell lines.. – for type 2 IHC

# Questions and/or comments



Thank You for the attention and.....